Pile Dynamics, Inc.

Transducer 172I

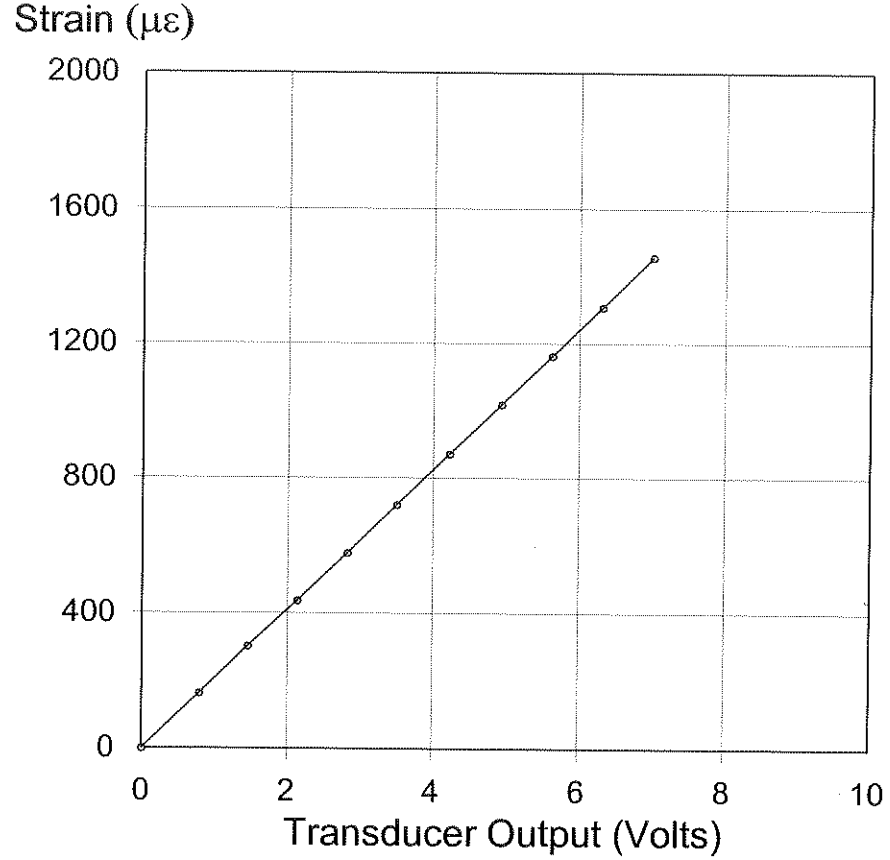

PDA Cal Factor (5.0 V) 103.8με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
163	0.78
301	1.45
436	2.13
576	2.81
719	3.50
870	4.22
1017	4.93
1164	5.62
1309	6.30
1458	7.01

Shunt (60.4 KΩ) 2.5 V

General Factor 360.3με/mV/V

Traceable to N.I.S.T.

Calibrated by: [signature]

Calibrated on: 25-Jun-2010

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? [X] yes [ ] no Smart Chip programmed by: G.P. on: 6-25-10 CRC value: E561