Pile Dynamics, Inc.

Transducer 185I

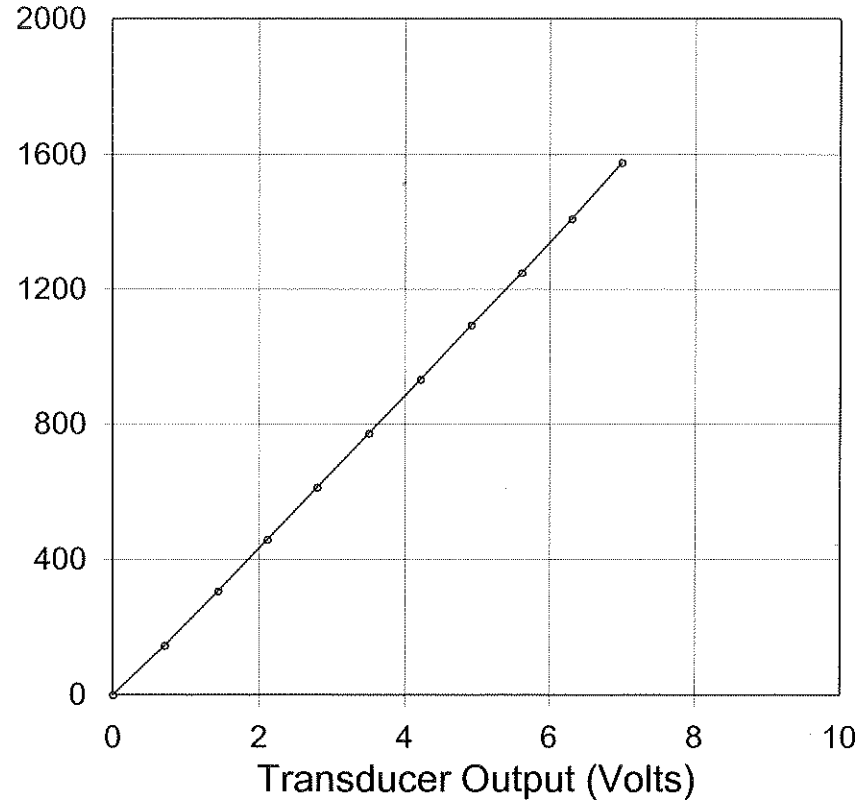

PDA Cal Factor (5.0 V) 112.9με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
147	0.70
305	1.43
457	2.11
611	2.79
772	3.50
932	4.21
1093	4.91
1249	5.61
1410	6.30
1578	6.99

Shunt (60.4 KΩ) 2.5 V

General Factor 391.9με/mV/V

Traceable to N.I.S.T.

Calibrated by:

Calibrated on: 25-Jun-2010

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? [X] yes [ ] no Smart Chip programmed by: G.P. on: 6-25-10 CRC value: CEEE