Pile Dynamics, Inc.

Transducer 223W

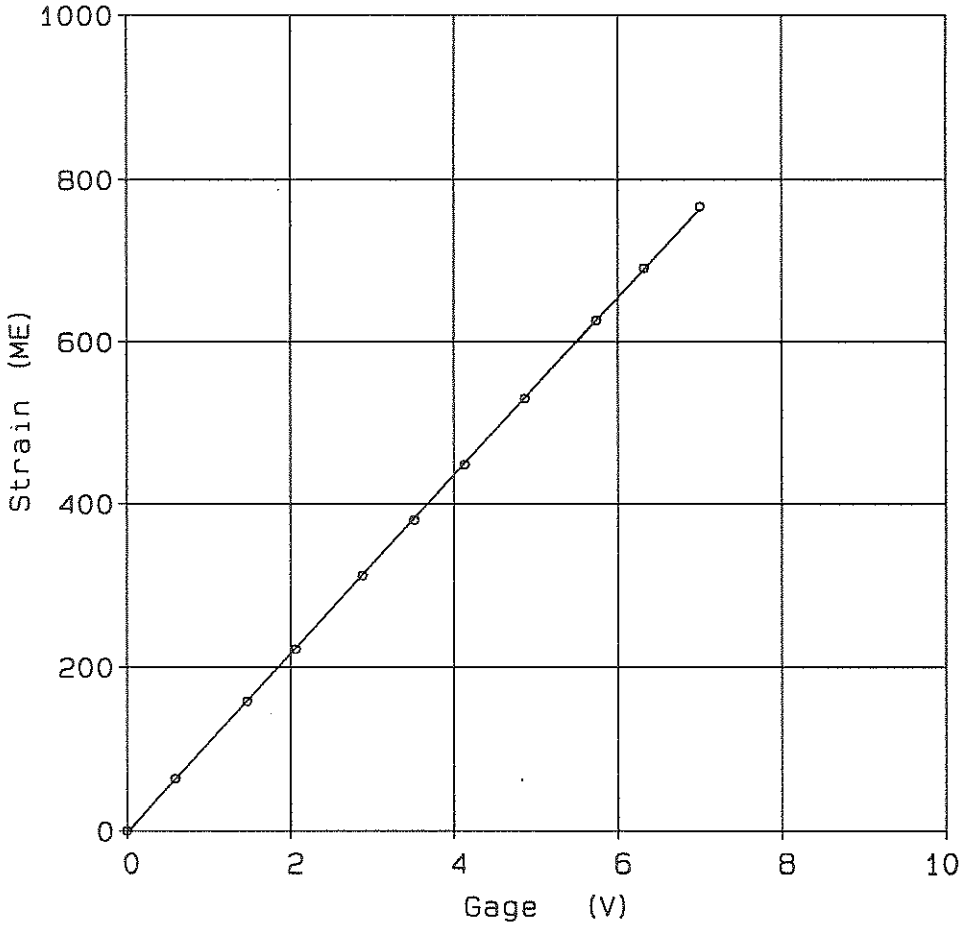

PDA Cal Factor = 109.5 ME/V
Shunt (60.4KO) = 5.0 V

General Factor = 380.3 ME/mV/V
Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
64	.60
159	1.47
222	2.06
313	2.89
381	3.52
449	4.13
530	4.88
627	5.74
691	6.33
767	7.01

Calibrated by: Jim Deutschendorff

Calibrated on: 01-Nov-94

Strain Transducer Calibration System - Version 1994-2