


Pile Dynamics Inc Transducer 236D

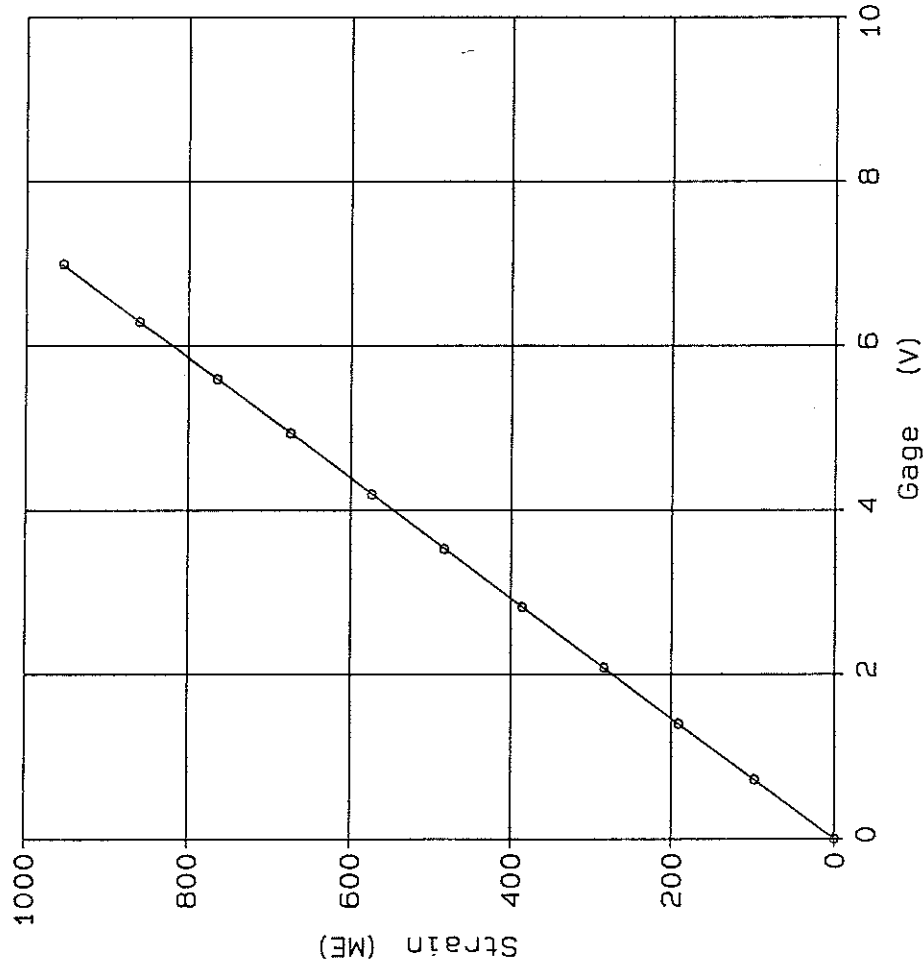

PDA Cal Factor = 136.8 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 475.2 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
98	.72
191	1.41
285	2.09
386	2.83
484	3.54
574	4.20
676	4.93
766	5.59
860	6.29
955	7.00

Calibrated by: Brent A. Smith

Calibrated on: 14-Oct-02