Pile Dynamics, Inc.
Transducer 239W

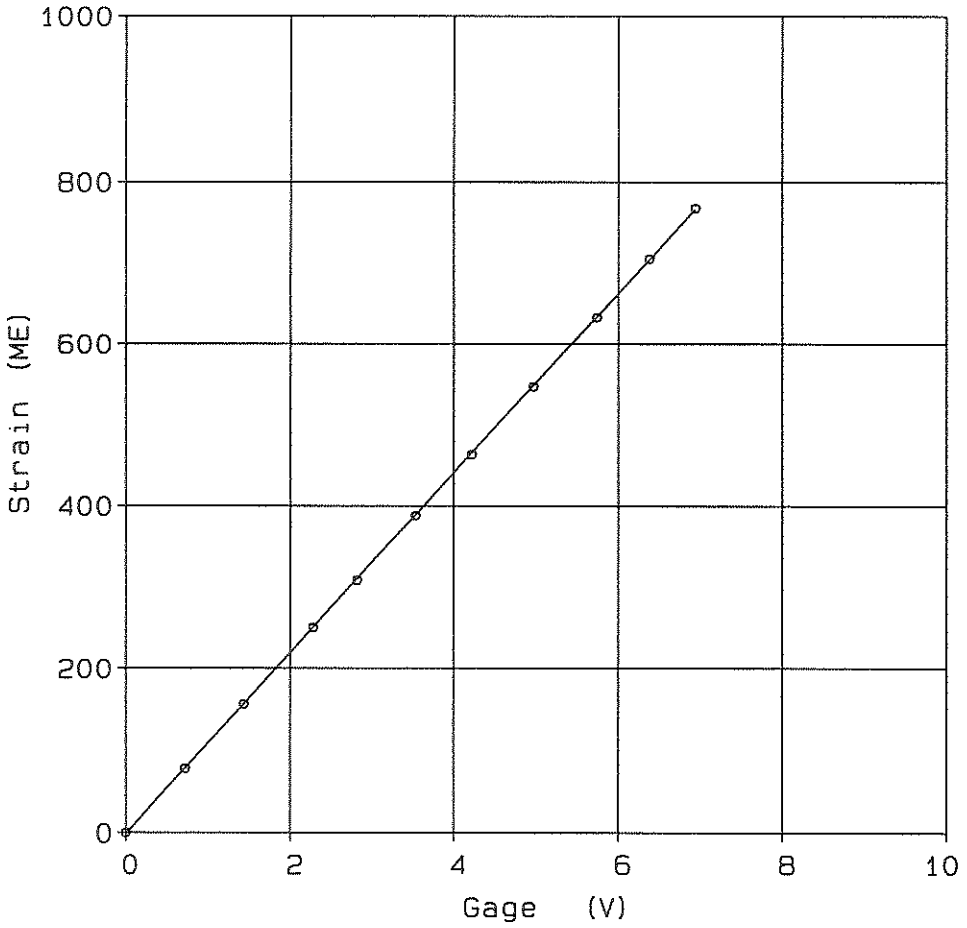

PDA Cal Factor = 110.8 ME/V
Shunt (60.4KO) = 5.0 V

General Factor = 384.7 ME/mV/V
Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
78	.72
156	1.44
250	2.29
309	2.82
389	3.54
464	4.22
548	4.98
634	5.74
706	6.39
769	6.95

Calibrated by: Jim Stentschneider

Calibrated on: 19-Dec-94

Strain Transducer Calibration System - Version 1994-2