


Pile Dynamics Inc Transducer 296M

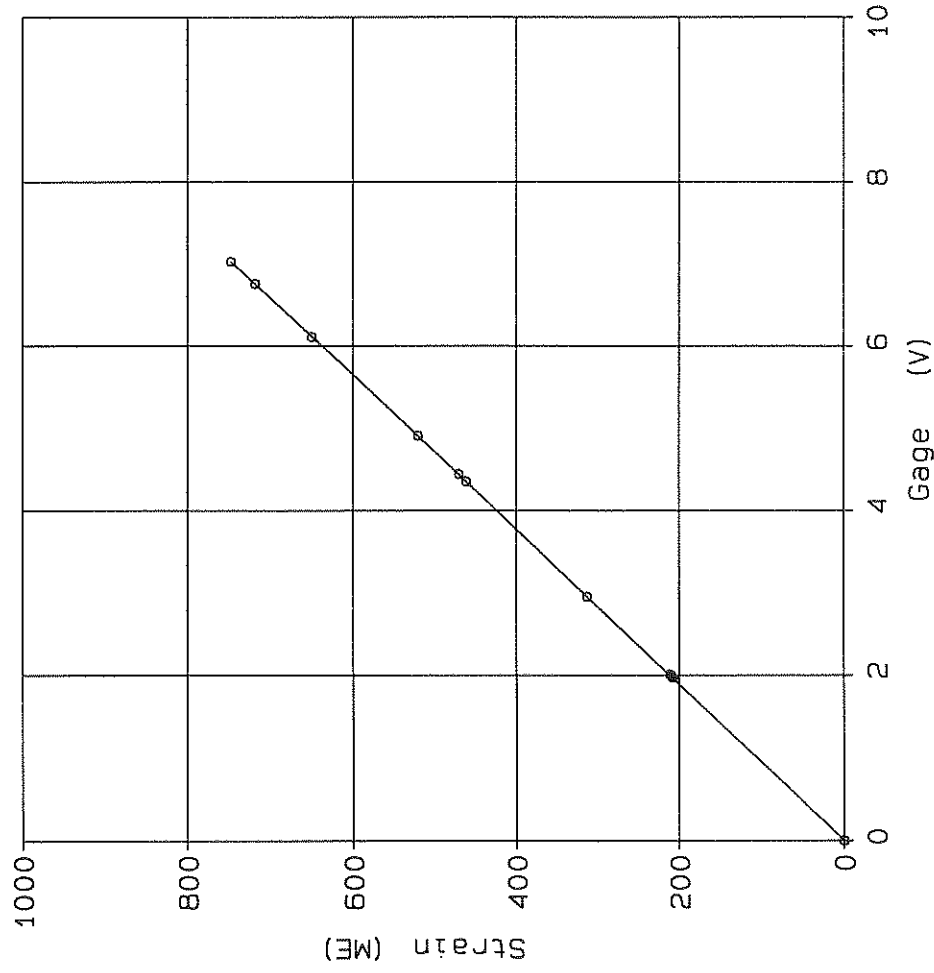

PDA Cal Factor = 106.5 ME/V
 Shunt (60.4KΩ) = 5.0 V

 General Factor = 369.8 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
212	2.01
210	1.99
209	1.98
313	2.96
462	4.36
471	4.45
522	4.91
650	6.12
719	6.76
748	7.03

Calibrated by: J. Pentel
 Calibrated on: 14-Jul-00