


Pile Dynamics Inc Transducer 297M

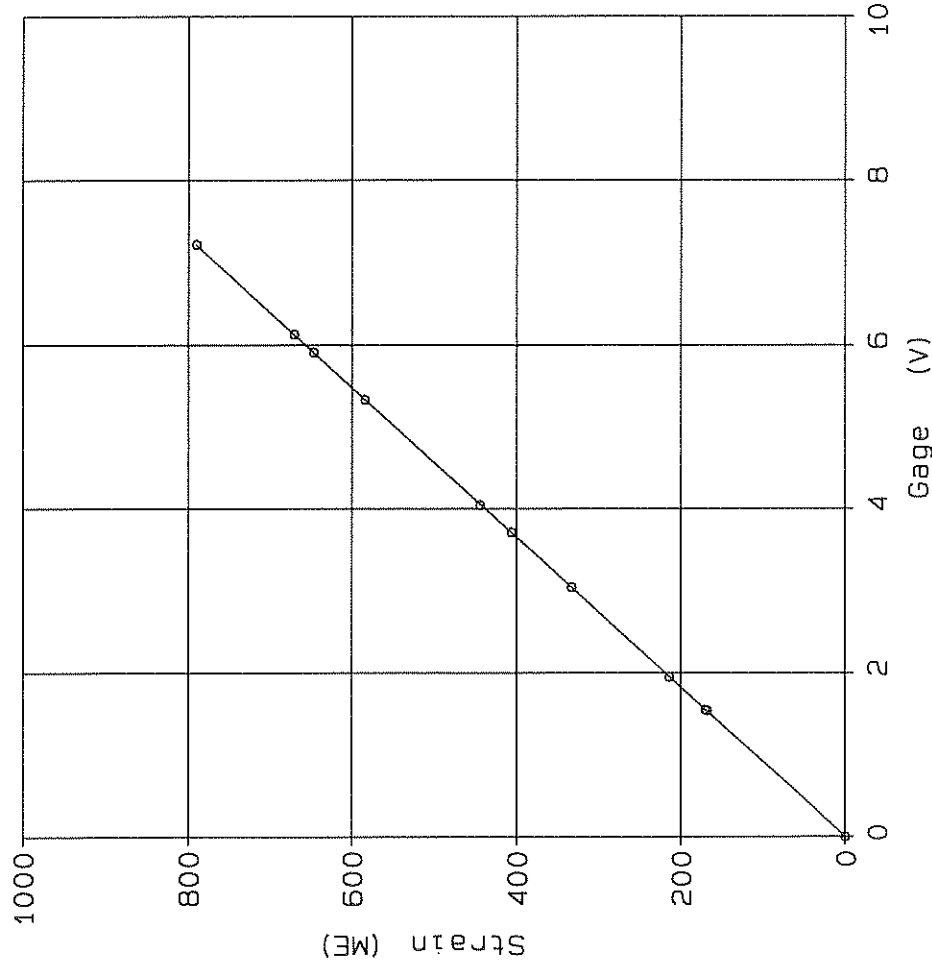

PDA Cal Factor = 109.5 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 380.2 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
170	1.56
169	1.54
214	1.96
334	3.05
407	3.71
444	4.05
585	5.34
648	5.91
672	6.13
790	7.22

Calibrated by: J. Donatelli
 Calibrated on: 21-Oct-99