Pile Dynamics, Inc.

Transducer 299W

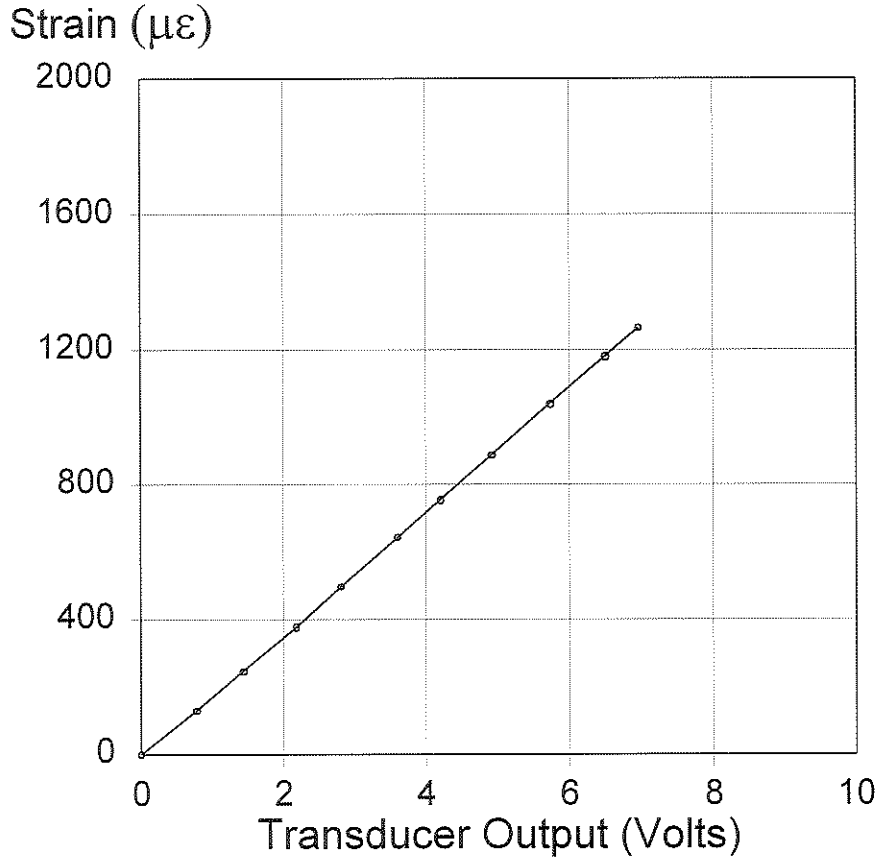

PDA Cal Factor 183.3με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
128	0.77
246	1.43
379	2.18
495	2.80
643	3.60
754	4.20
887	4.91
1040	5.73
1181	6.50
1265	6.96

Shunt (60.4 KΩ) 5.0 V

General Factor 636.5με/mV/V

Traceable to N.I.S.T.

Calibrated by: Fred Hvorslev

Calibrated on: 02-Feb-2004

Strain Transducer Calibrator System 2004 Version 1.2