
Pile Dynamics, Inc.

Transducer 302W

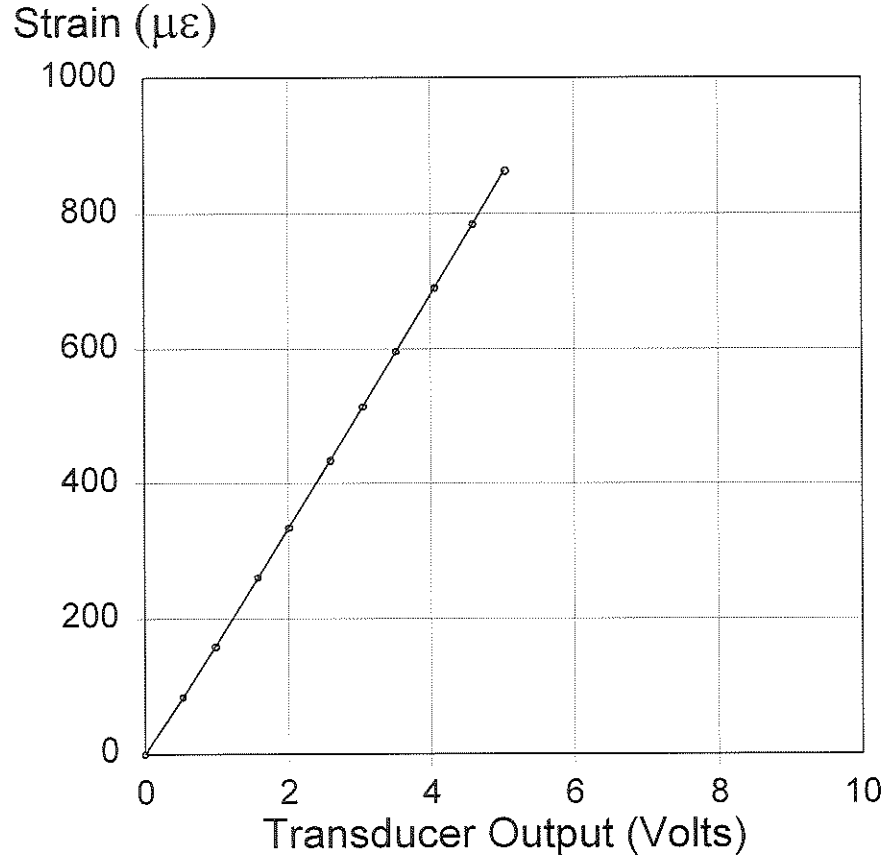

PDA Cal Factor 172.4με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
84	0.53
159	0.98
260	1.57
334	2.00
435	2.59
514	3.04
596	3.51
691	4.05
785	4.58
864	5.03

Shunt (60.4 KΩ) 5.0 V

General Factor 598.7με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Deutsch

Calibrated on: 26-Jan-2004

Strain Transducer Calibrator System 2004 Version 1.2