
Pile Dynamics, Inc.

Transducer 305W

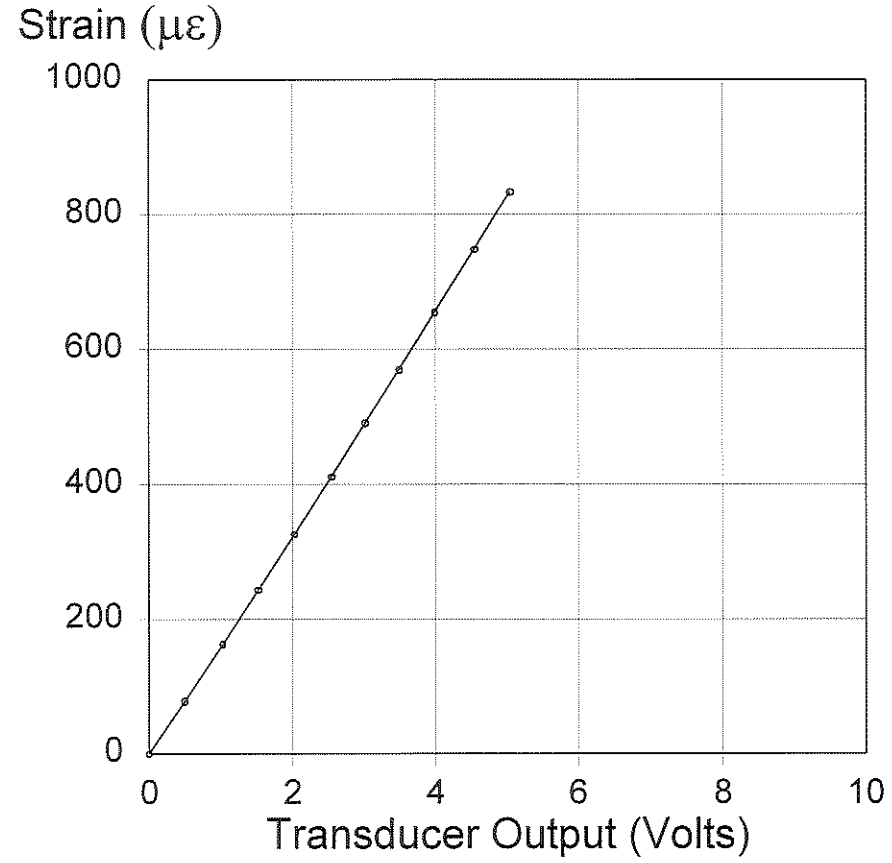

PDA Cal Factor 165.8με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
79	0.50
163	1.03
243	1.52
325	2.01
410	2.53
491	3.01
570	3.48
655	3.99
748	4.53
833	5.03

Shunt (60.4 KΩ) 5.0 V

General Factor 575.8με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Deutsch

Calibrated on: 28-Jan-2004

Strain Transducer Calibrator System 2004 Version 1.2