Pile Dynamics, Inc.

Transducer 317W

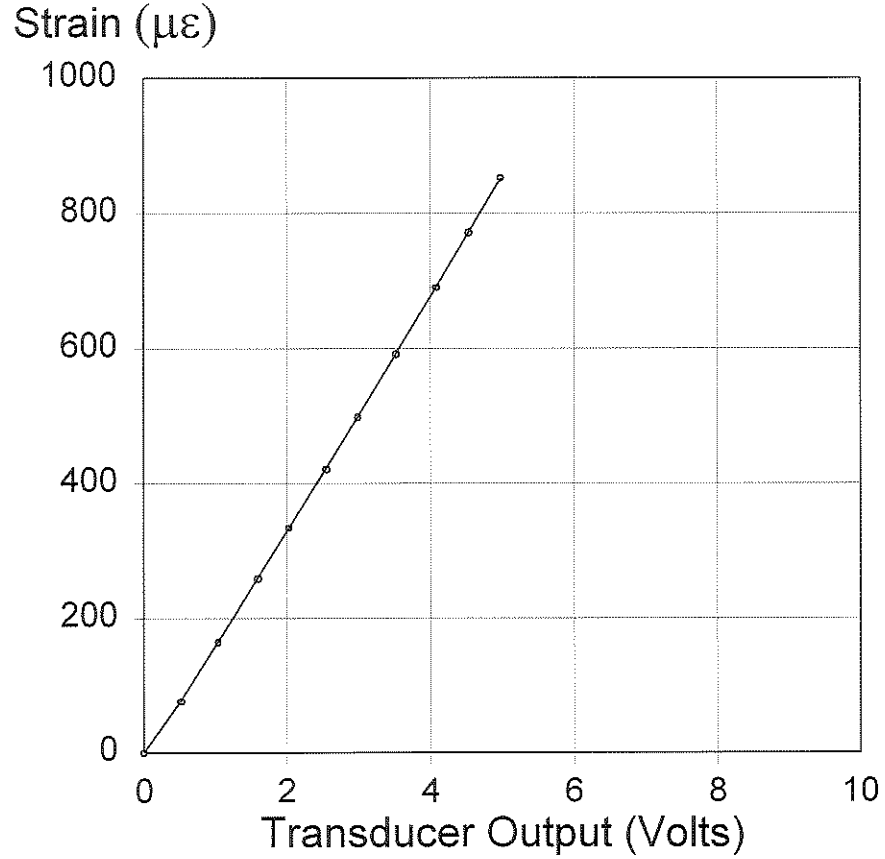

PDA Cal Factor 172.3με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
77	0.50
165	1.04
258	1.58
332	2.02
422	2.54
499	2.98
592	3.51
690	4.06
773	4.53
853	4.97

Shunt (60.4 KΩ) 5.0 V

General Factor 598.2με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Tuttle

Calibrated on: 28-Jan-2004

Strain Transducer Calibrator System 2004 Version 1.2