Pile Dynamics, Inc.

Transducer 320W

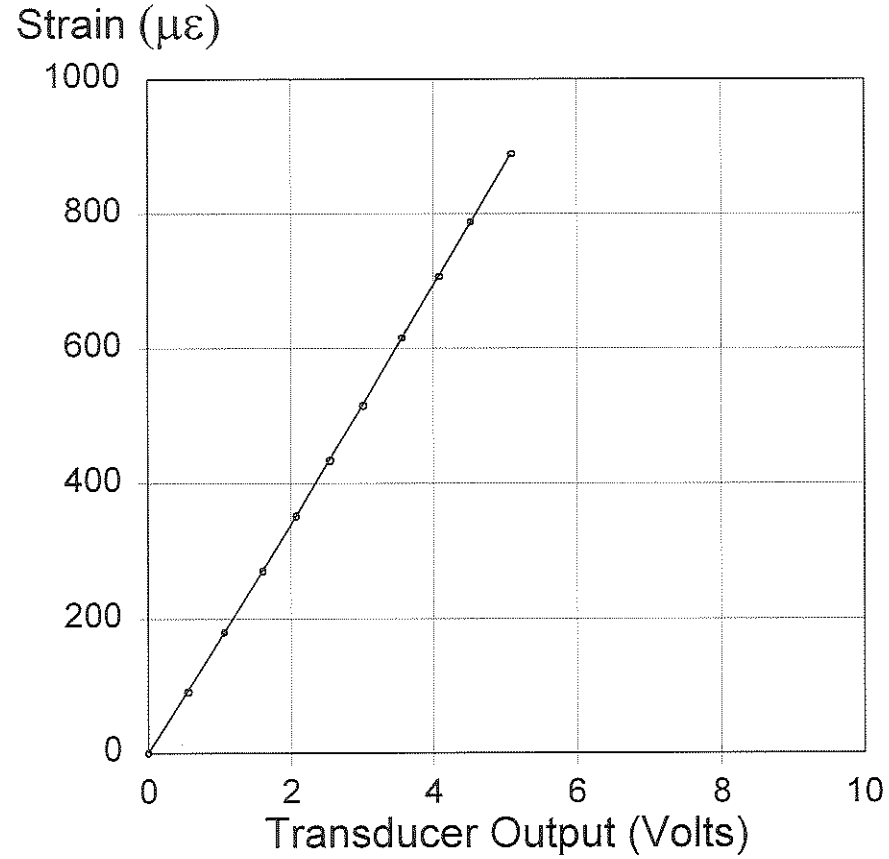

PDA Cal Factor 175.6με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
91	0.55
180	1.07
271	1.60
353	2.07
435	2.54
516	3.00
615	3.55
708	4.07
788	4.51
889	5.07

Shunt (60.4 KΩ) 5.0 V

General Factor 609.7με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Deutsch

Calibrated on: 28-Jan-2004

Strain Transducer Calibrator System 2004 Version 1.2