Pile Dynamics, Inc.

Transducer 337W

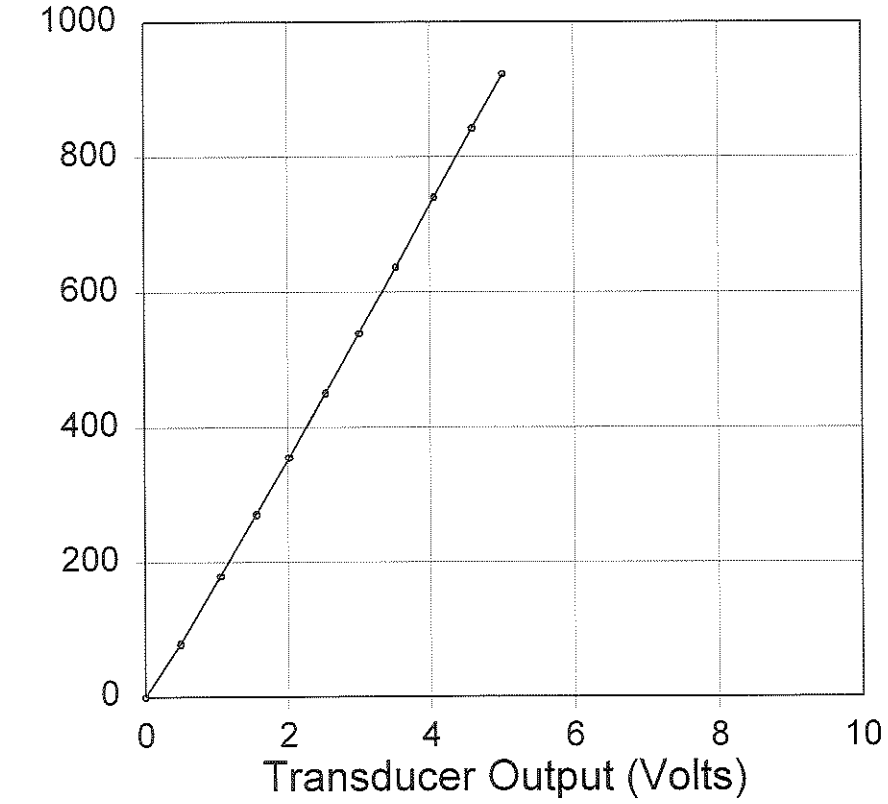

PDA Cal Factor 185.5με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
79	0.49
178	1.05
271	1.55
355	2.01
451	2.53
538	2.99
637	3.52
740	4.06
842	4.59
923	5.01

Shunt (60.4 KΩ) 5.0 V

General Factor 644.0με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Davis

Calibrated on: 28-Jan-2004

Strain Transducer Calibrator System 2004 Version 1.2