
Pile Dynamics, Inc.

Transducer 355W

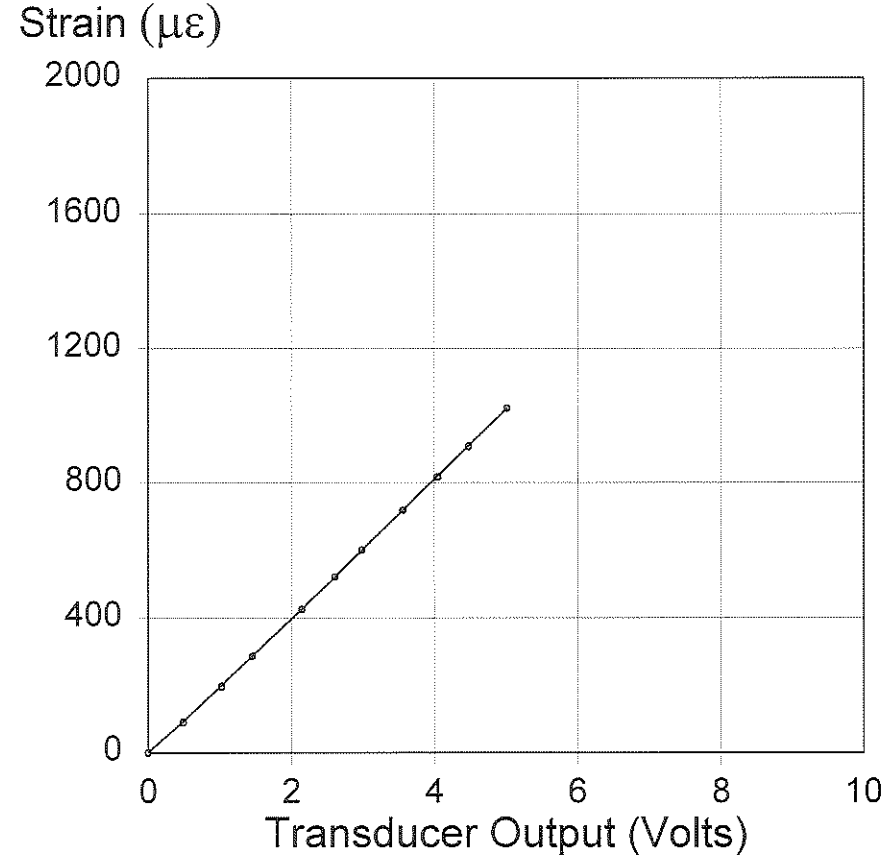

PDA Cal Factor 204.8με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
92	0.49
199	1.02
287	1.45
426	2.14
520	2.60
600	2.99
718	3.55
818	4.03
910	4.47
1023	5.01

Shunt (60.4 KΩ) 5.0 V

General Factor 711.2με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Newlin

Calibrated on: 27-Jan-2004

Strain Transducer Calibrator System 2004 Version 1.2