



Pile Dynamics, Inc.


Pile Dynamics, Inc.

Transducer 610C

Strain ($\mu\epsilon$)

PDA Cal Factor

113.6 $\mu\epsilon/V$

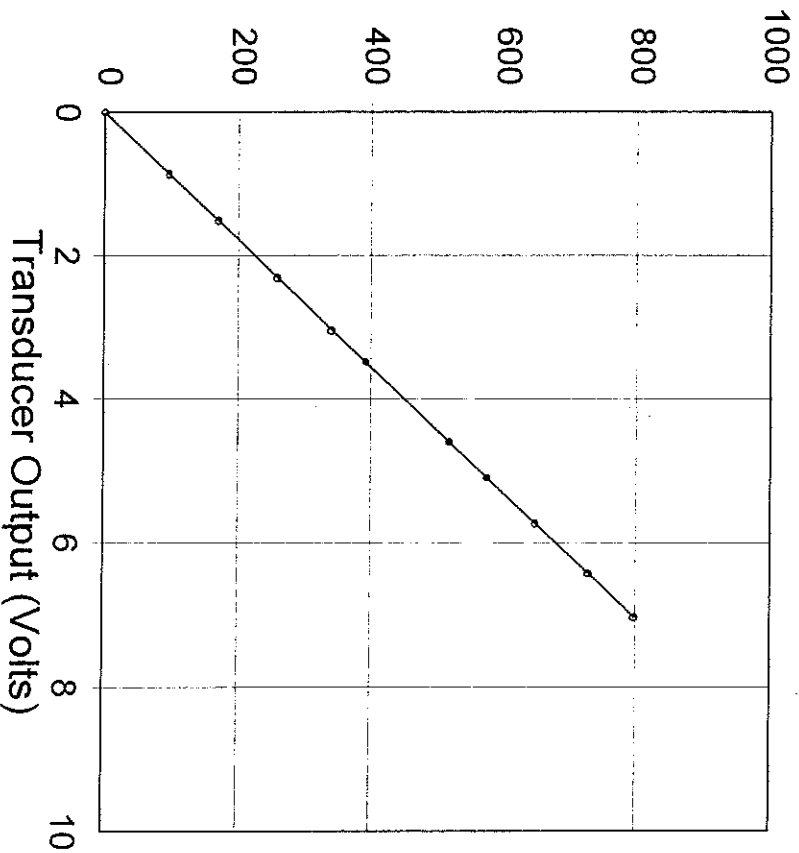

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
96	0.85
169	1.50
258	2.30
341	3.03
391	3.48
519	4.60
577	5.10
648	5.72
729	6.43
799	7.03

Shunt (60.4 K Ω)
General Factor

5.0 V
394.5 $\mu\epsilon/mV/V$

Calibrated by:
Calibrated on:

20-JUL-2004