


PILE DYNAMICS, INC.

6/3/86 CAL

GAGE NO. 615 C

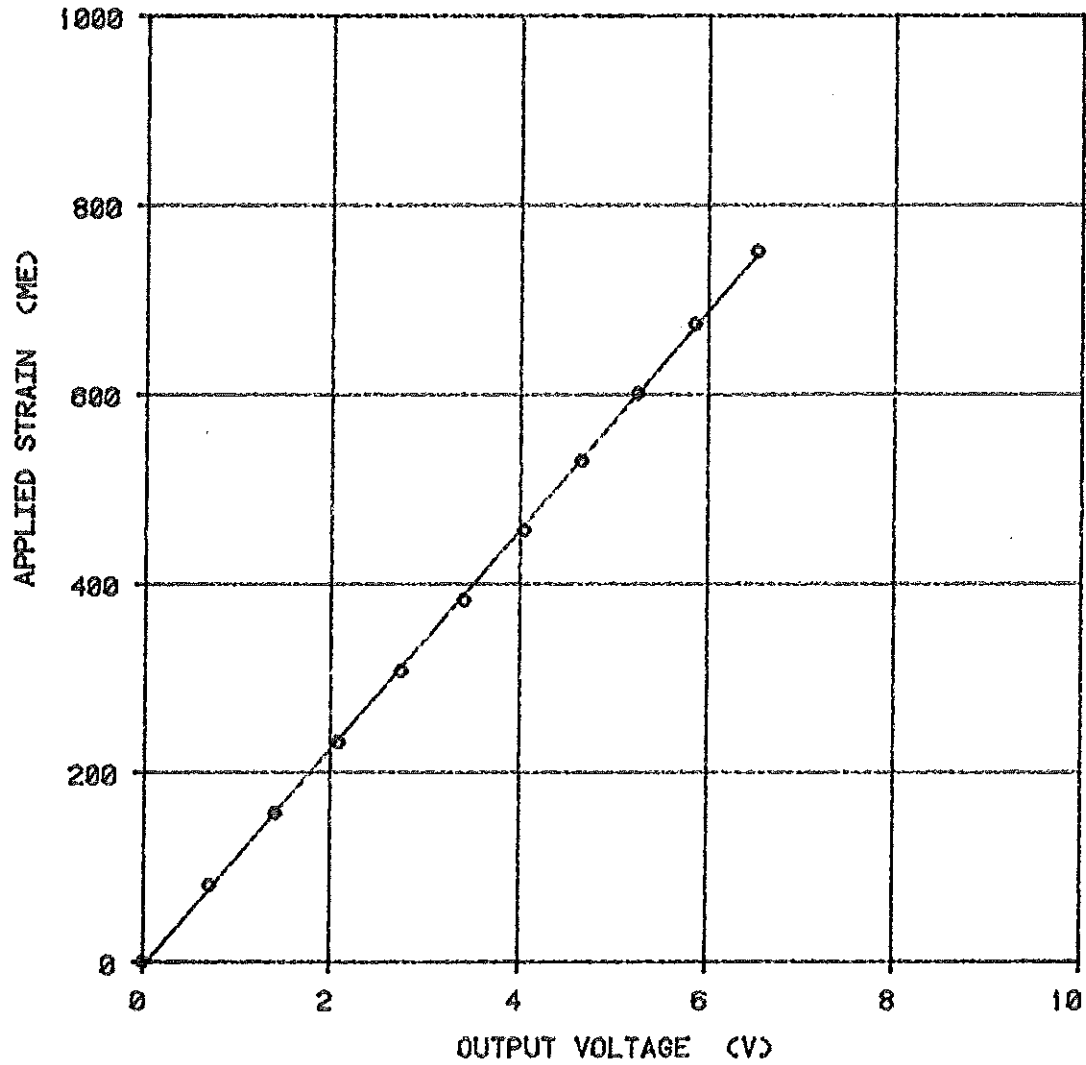

INIT

6/3/86 CAL
GAGE NO. 615C

NO.	APPLD. STRAIN ME	GAGE VOLTAGE V
1	0.000	0.000
2	81.139	0.718
3	157.250	1.414
4	232.059	2.088
5	307.351	2.749
6	382.904	3.405
7	456.149	4.041
8	530.548	4.655
9	601.595	5.256
10	674.393	5.870
11	751.510	6.525

GAGE CALIBRATION FACTOR= 115.340 ME/V

GAGE REF. SHUNT (60.4K0)= 5.000 VOLTS

OFFSET = -5.3697 CORRELATION COEFFICIENT = 0.9999

VALUES ARE AVERAGED