Pile Dynamics, Inc.

Transducer 744W

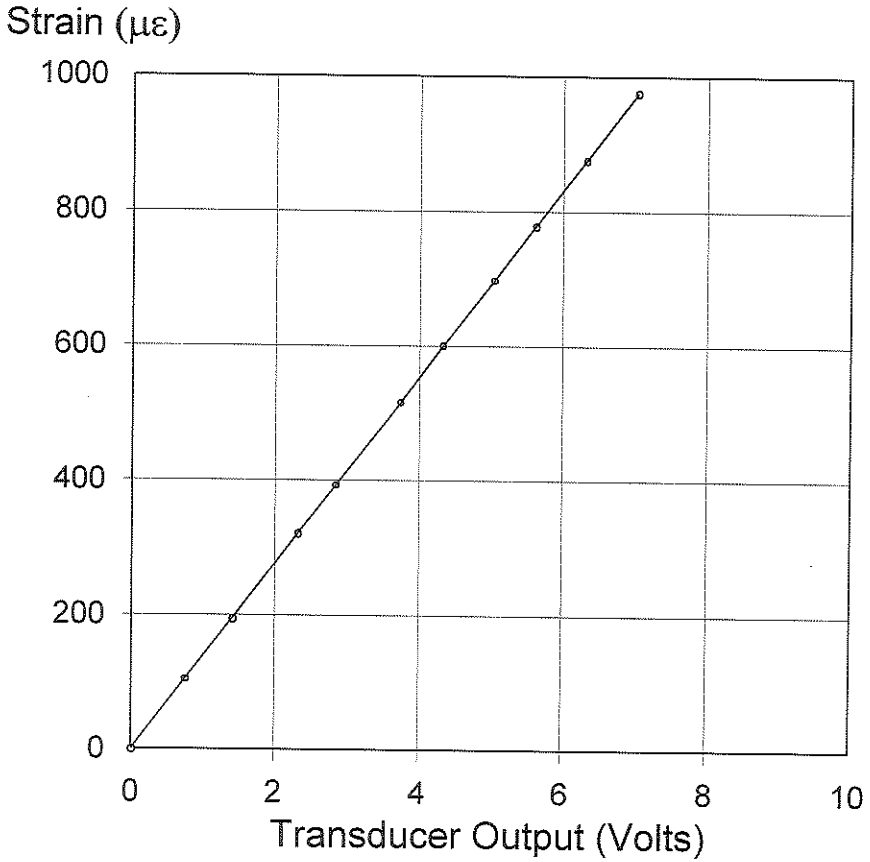

PDA Cal Factor 138.9με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
105	0.75
194	1.41
321	2.32
392	2.83
516	3.73
600	4.32
697	5.03
779	5.61
877	6.32
977	7.03

Shunt (60.4 KΩ) 5.0 V

General Factor 482.4με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Cantelli

Calibrated on: 22-Dec-2004

Strain Transducer Calibrator System 2004 Version 1.2