Pile Dynamics, Inc.

Transducer 745W

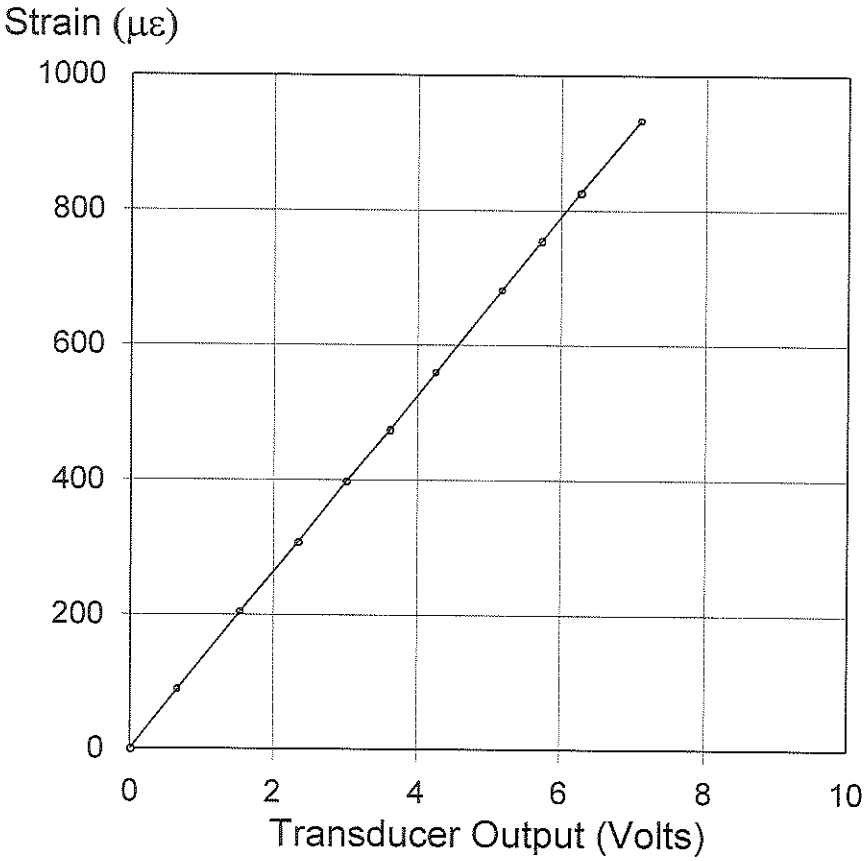

PDA Cal Factor 131.7με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
89	0.66
204	1.53
307	2.33
398	3.00
475	3.61
559	4.25
681	5.16
755	5.72
827	6.26
934	7.10

Shunt (60.4 KΩ) 5.0 V

General Factor 457.4με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Newton

Calibrated on: 17-Jan-2005

Strain Transducer Calibrator System 2004 Version 1.2