Pile Dynamics, Inc.

Transducer 748W

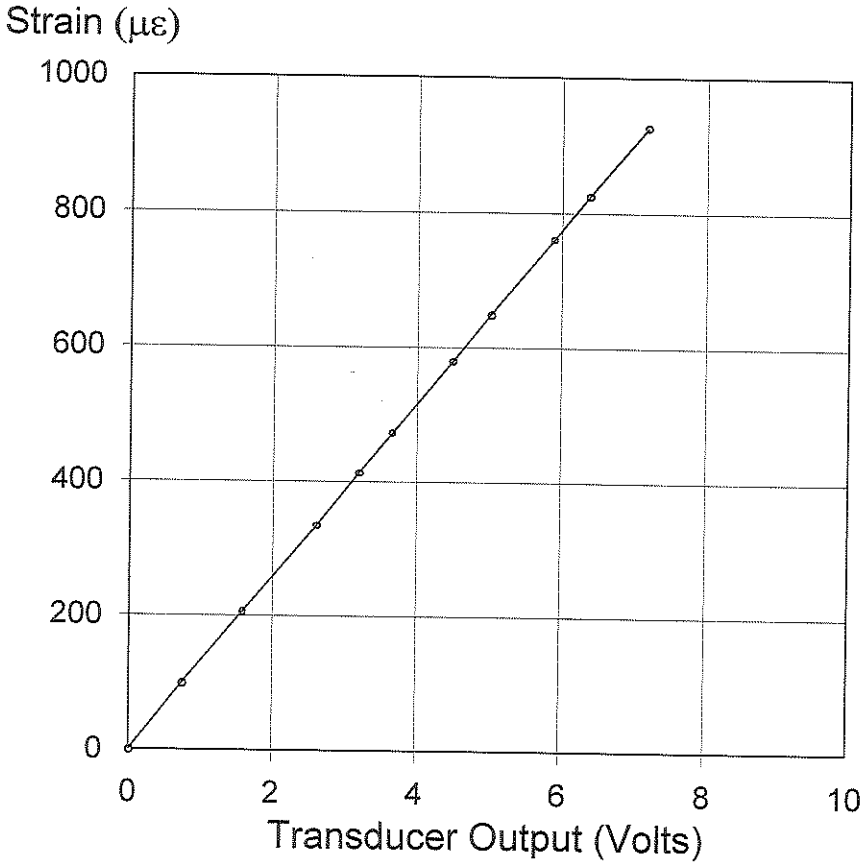

PDA Cal Factor 129.0με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
100	0.74
206	1.58
334	2.59
412	3.19
472	3.65
579	4.49
649	5.01
760	5.88
825	6.37
927	7.18

Shunt (60.4 KΩ) 5.0 V

General Factor 448.0με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Rausche

Calibrated on: 23-Dec-2004

Strain Transducer Calibrator System 2004 Version 1.2