Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 752A
PDI Gage Factor: 94.6
Mean Linear Correlation Coefficient: 0.999938

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2316.7	-7.062	508.3	1.628
-1808.3	-5.474	891.7	2.820
-1308.3	-3.961	1200.0	3.741
-858.3	-2.558	1508.3	4.654
-425.0	-1.273	1800.0	5.503
-75.0	-0.164	1983.3	6.036
208.3	0.707		

Calibration Curve

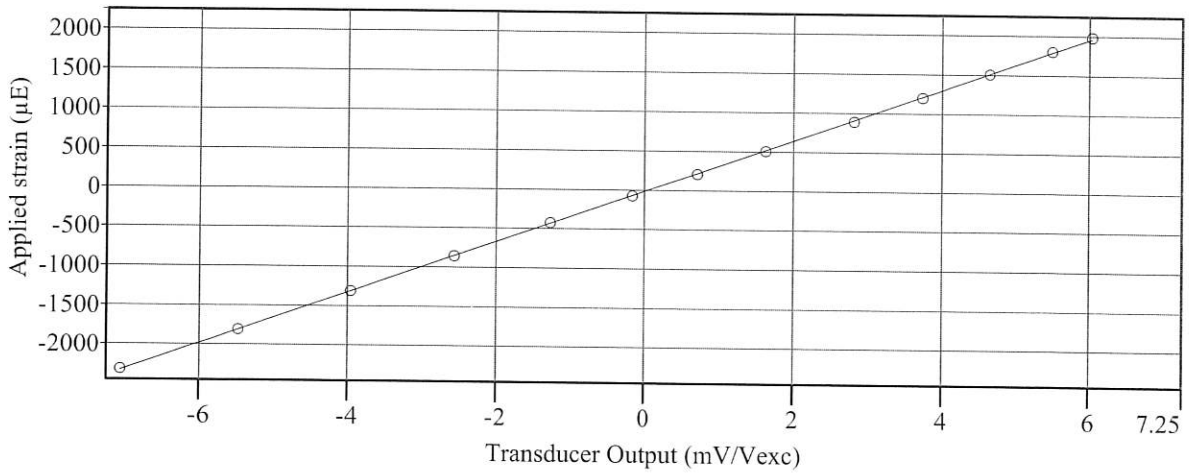

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: 752A
Calibration Date: JUN 2 7 2025

Pile Dynamics, Inc.