




Pile Dynamics, Inc.

Transducer 921W

Strain ($\mu\epsilon$)

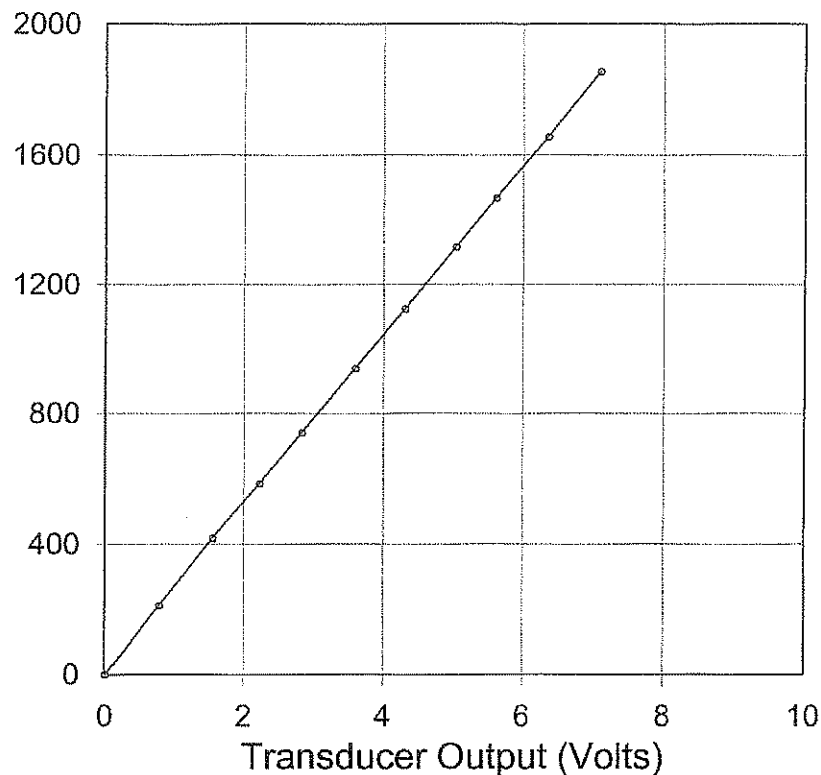

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

PDA Cal Factor (5.0 V)

130.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
214	0.77
418	1.54
586	2.22
740	2.83
940	3.59
1124	4.30
1317	5.03
1469	5.61
1658	6.35
1855	7.09

Shunt (60.4 K Ω)

2.5 V

General Factor

451.6 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

[Signature]
26-Jan-2010