




Pile Dynamics, Inc.

Transducer 923W

Strain ($\mu\epsilon$)

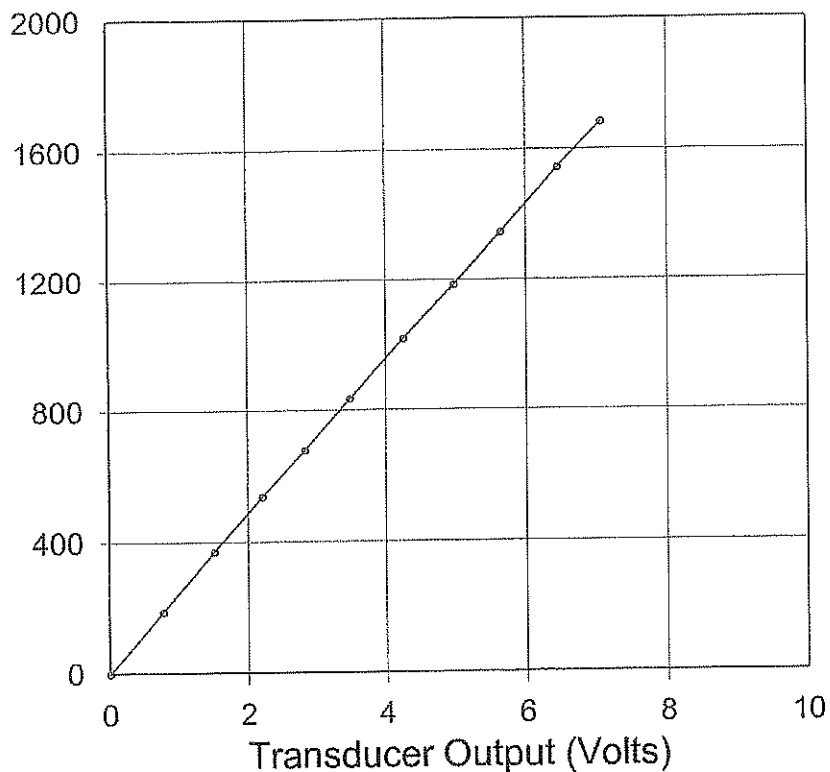

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

PDA Cal Factor (5.0 V)

118.8 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
189	0.76
371	1.50
535	2.22
675	2.83
834	3.48
1019	4.25
1185	4.98
1348	5.65
1544	6.45
1685	7.07

Shunt (60.4 K Ω)

2.5 V

General Factor

412.6 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

James Dantley
17-Feb-2010