




Pile Dynamics, Inc.

Transducer 924W

Strain ($\mu\epsilon$)

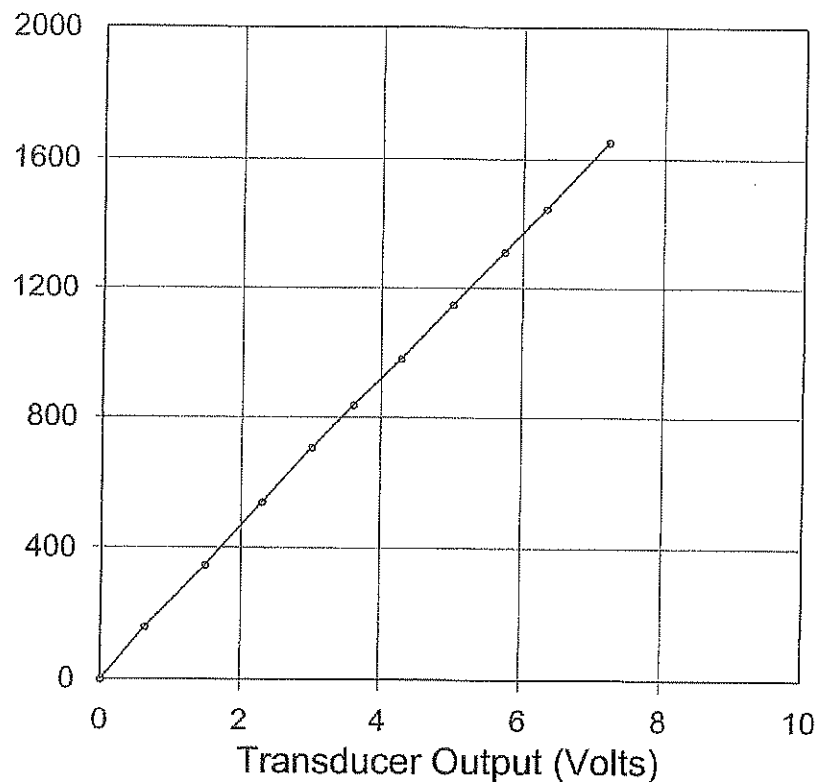

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

PDA Cal Factor (5.0 V)

113.8 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
159	0.62
347	1.48
540	2.30
706	3.00
837	3.60
980	4.28
1148	5.01
1313	5.73
1446	6.32
1653	7.20

Shunt (60.4 K Ω)

2.5 V

General Factor

395.0 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

17-Feb-2010