




Pile Dynamics, Inc.

Transducer 926W

Strain ($\mu\epsilon$)

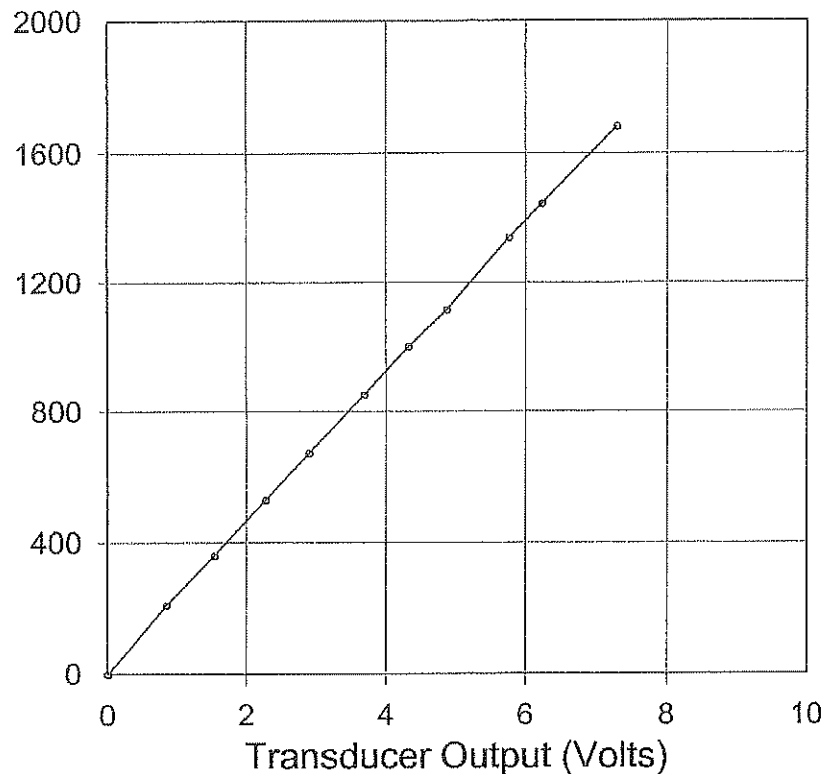

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

PDA Cal Factor (5.0 V) 115.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
212	0.84
361	1.53
529	2.27
672	2.90
851	3.69
1000	4.32
1115	4.87
1341	5.76
1446	6.23
1683	7.30

Shunt (60.4 K Ω)

2.5 V

General Factor

399.6 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

James C. Smith
17-Feb-2010