




Pile Dynamics, Inc.

Transducer 927W

Strain ($\mu\epsilon$)

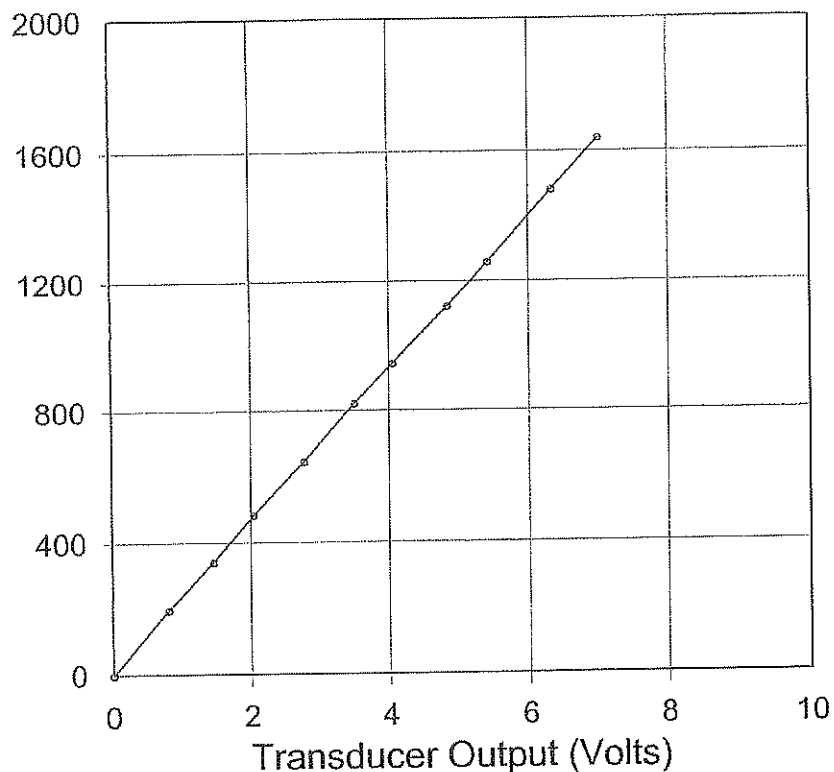

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

PDA Cal Factor (5.0 V)

116.6 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
198	0.80
340	1.45
481	2.04
644	2.77
821	3.50
945	4.05
1122	4.83
1258	5.40
1483	6.33
1640	7.01

Shunt (60.4 K Ω)

2.5 V

General Factor

404.8 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

James A. Smith
17-Feb-2010