




Pile Dynamics, Inc.

Transducer 929W

Strain ($\mu\epsilon$)

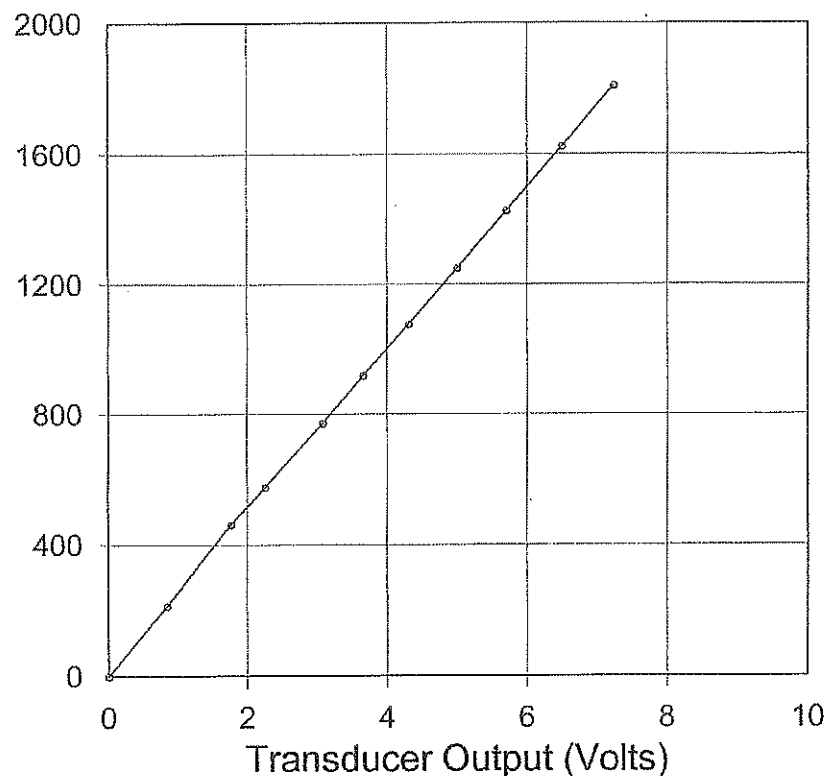

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

PDA Cal Factor (5.0 V) 124.5 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
214	0.84
462	1.76
575	2.25
773	3.07
920	3.65
1076	4.30
1251	5.00
1428	5.71
1624	6.49
1810	7.23

Shunt (60.4 K Ω) 2.5 V

General Factor 432.2 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

James A. Smith
17-Feb-2010