




Pile Dynamics, Inc.

Transducer 930W

Strain ($\mu\epsilon$)

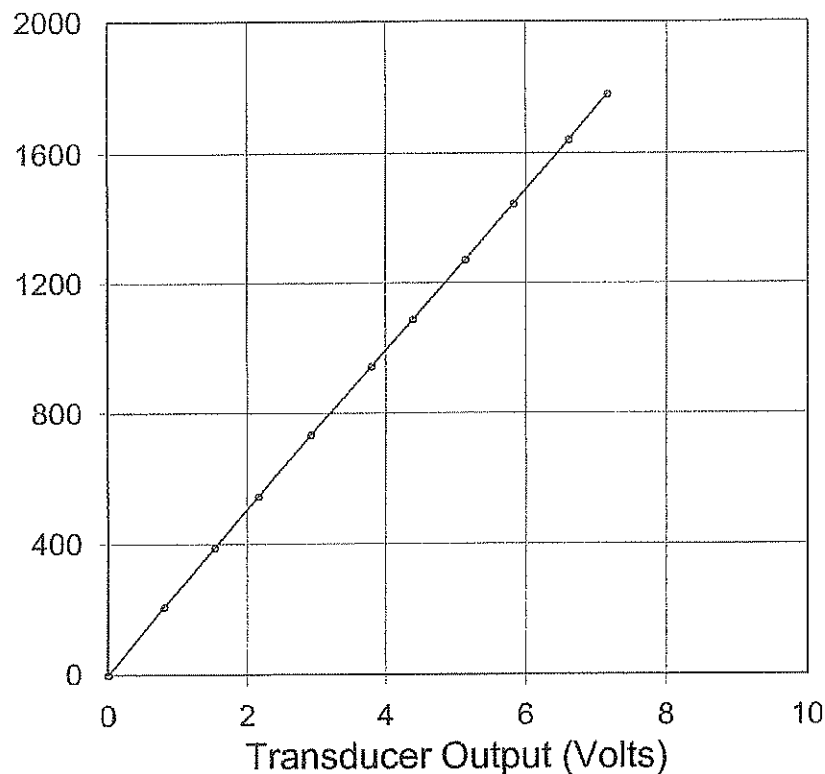

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

PDA Cal Factor (5.0 V)

123.5 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
209	0.80
389	1.52
545	2.16
734	2.92
943	3.79
1088	4.39
1272	5.14
1444	5.82
1642	6.61
1780	7.16

Shunt (60.4 K Ω)

2.5 V

General Factor

428.7 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

James P. O'Connell
17-Feb-2010