




Pile Dynamics, Inc.

Transducer 931W

Strain ($\mu\epsilon$)

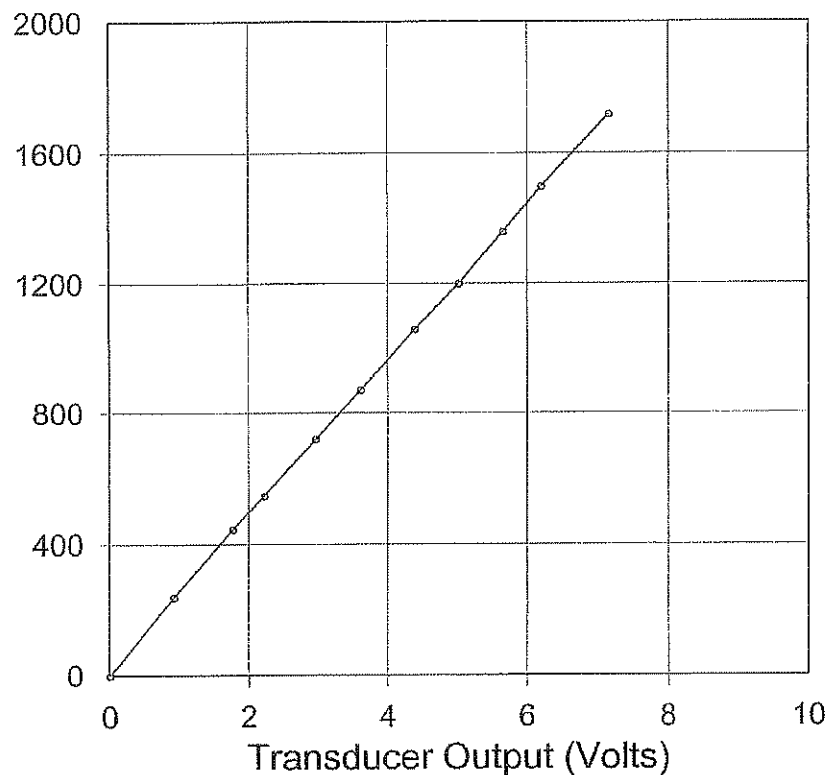

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

PDA Cal Factor (5.0 V)

119.3 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
239	0.91
444	1.76
547	2.22
720	2.96
872	3.62
1060	4.39
1200	5.02
1361	5.65
1499	6.20
1720	7.15

Shunt (60.4 K Ω)

2.5 V

General Factor

414.3 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

James R. Smith
17-Feb-2010