


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

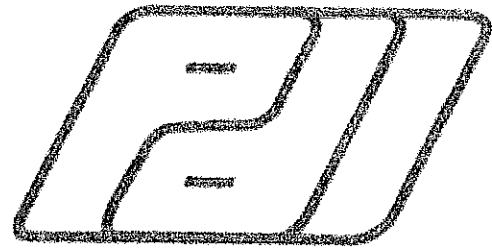

Serial No: K14429 Temperature: 22.6 °C
 Model: KICHER PR Humidity: 26%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

344.5 mv/5000g
 (68.9 μ v/g)
 R²: 0.999953 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
 971 g's/volt
 Ref Acc 2: 78268! Cal on: 11Jan2024
 986 g's/volt


Operator: William Johnson

William Johnson
 Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: **JUN 20 2025**

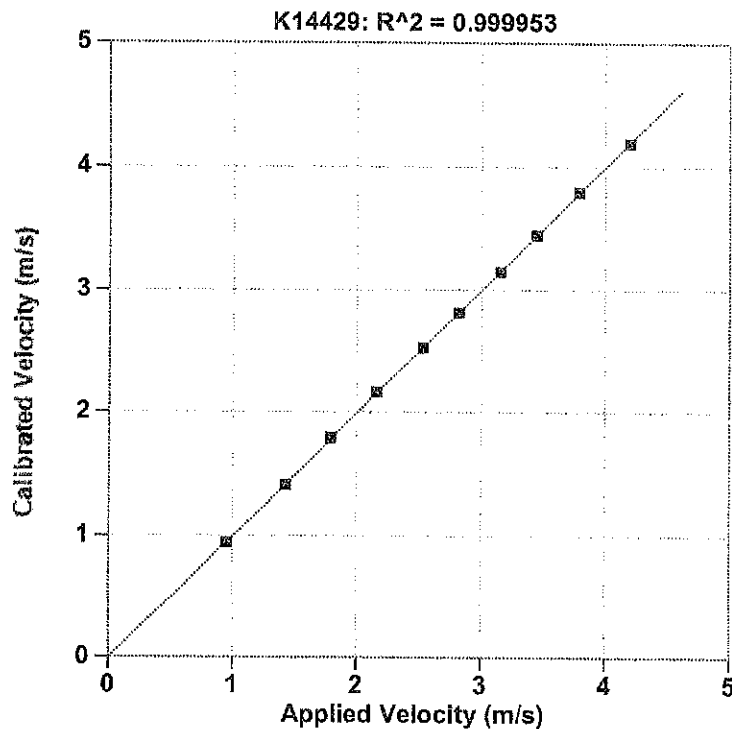

Reference Velocity	S/N K14429 Velocity
m/s	m/s
0.957	0.947
1.421	1.415
1.787	1.794
2.156	2.165
2.537	2.532
2.821	2.820
3.154	3.148
3.445	3.452
3.793	3.800
4.199	4.192

Maximum Acceleration: 914 g's