

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K14490 Temperature: 22.1 °C

Model: KICHER PR Humidity: 26%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

375.7 mv/5000g

(75.1 μ v/g)

R²: 0.999912 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt

Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: **JUN 20 2025**

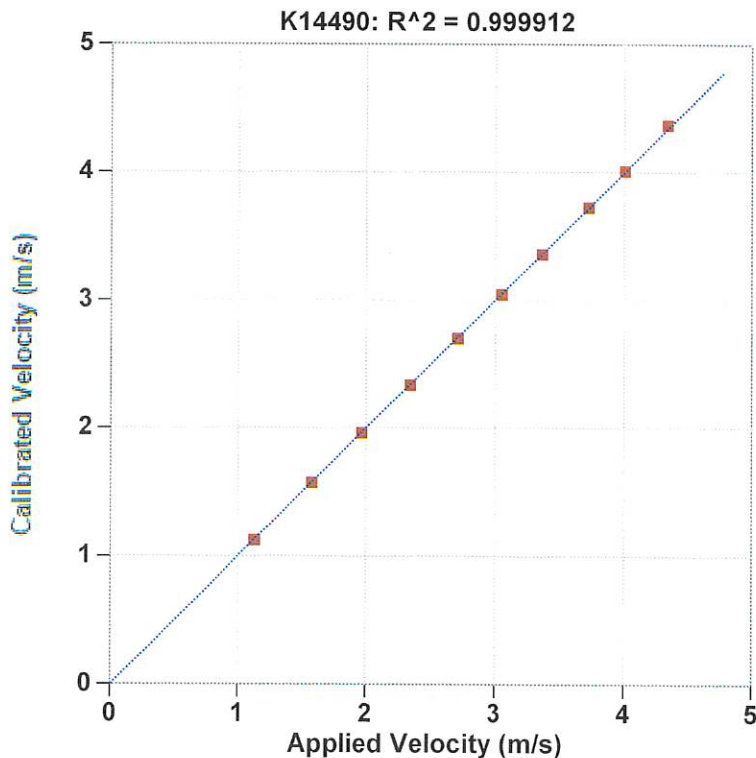

Reference Velocity	S/N K14490 Velocity
m/s	m/s
1.128	1.123
1.573	1.573
1.968	1.958
2.339	2.332
2.706	2.698
3.050	3.042
3.361	3.355
3.723	3.722
4.006	4.008
4.343	4.367
Maximum Acceleration: 950 g's	