Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K14697	**Temperature:**	25.5 °C
Model:	KICHER PR	**Humidity:**	71%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	78268! 986 g's/volt	**Cal on:**	11Jan2024
Ref Acc 2:	78270! 971 g's/volt	**Cal on:**	11Jan2024

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR


439.5 mv/5000g
(87.9 µv/g)
R^2: 0.999906 [Chip programmed]

Operator:

Signed

Calibration valid 2 years

From: JUN 25 2025

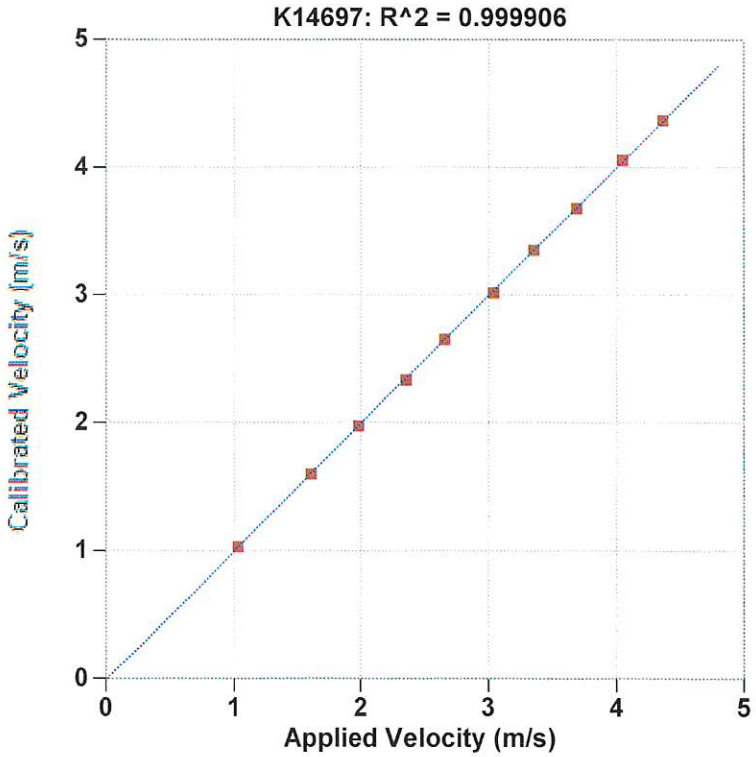

Reference Velocity	S/N K14697 Velocity
m/s	m/s
1.030	1.036
1.608	1.603
1.981	1.979
2.355	2.338
2.654	2.656
3.038	3.020
3.355	3.356
3.686	3.683
4.046	4.063
4.362	4.370

Maximum Acceleration: 949 g's