

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: LW525808 Temperature: 21.1 °C

Model: PIT ACC Humidity: 38%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

9.7 g's/volt

R²: 0.999923 [Chip programmed]

Operator: William Johnson

Signed


Calibration valid 2 years

From: JUN 18 2025

Ref Acc 1: LW503311! Cal on: 31Jan2024
10 g's/volt

Ref Acc 2: LW503313! Cal on: 31Jan2024
10 g's/volt

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

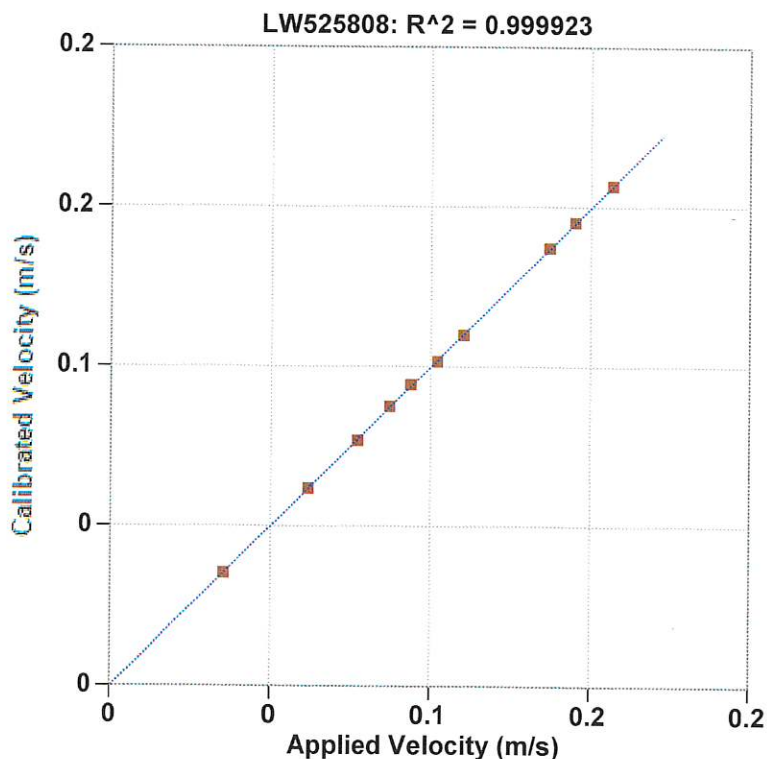

Reference Velocity	S/N LW525808 Velocity
m/s	m/s
0.035	0.035
0.062	0.062
0.077	0.077
0.087	0.088
0.094	0.094
0.102	0.102
0.110	0.110
0.137	0.137
0.145	0.145
0.157	0.157

Maximum Acceleration: 18 g's