


Pile Dynamics, Inc. Transducer 454H

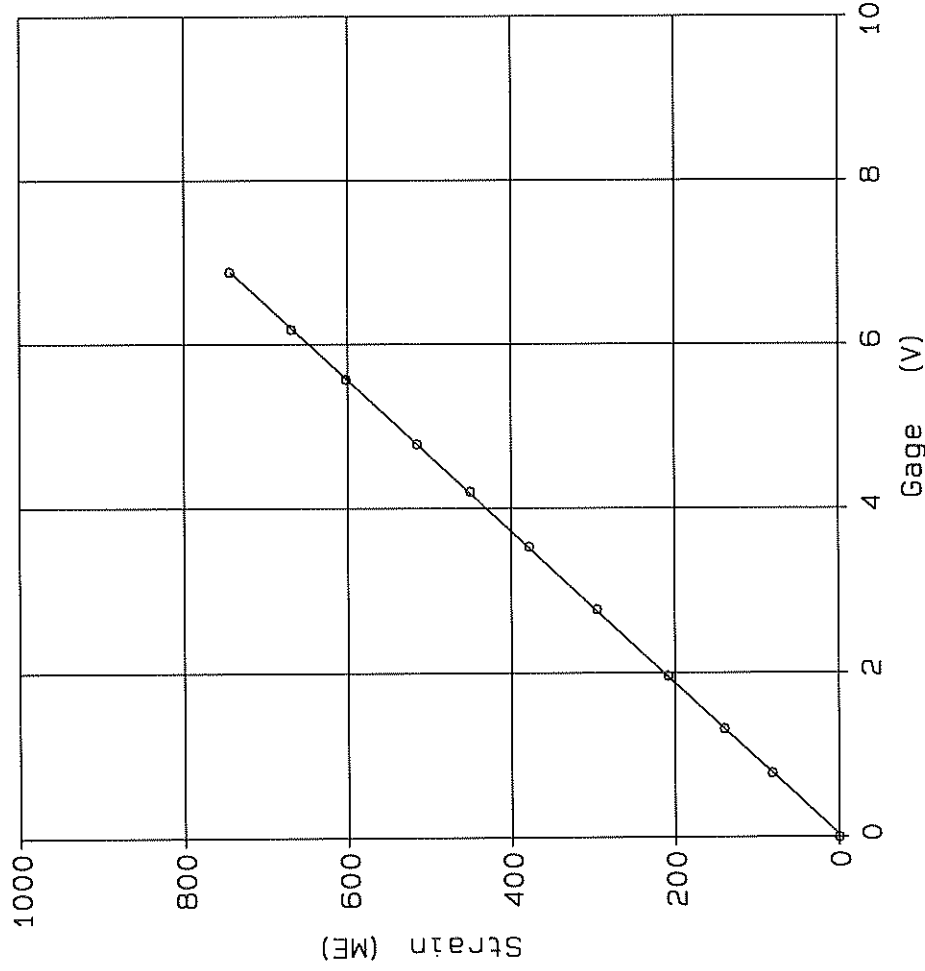

PDA Cal Factor = 108.5 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 376.8 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
83	.79
141	1.33
208	1.97
296	2.77
378	3.53
450	4.20
515	4.78
603	5.58
669	6.18
745	6.88

Calibrated by: J. S. Dunkel
 Calibrated on: 11-Jan-96