Pile Dynamics, Inc.

Transducer 479

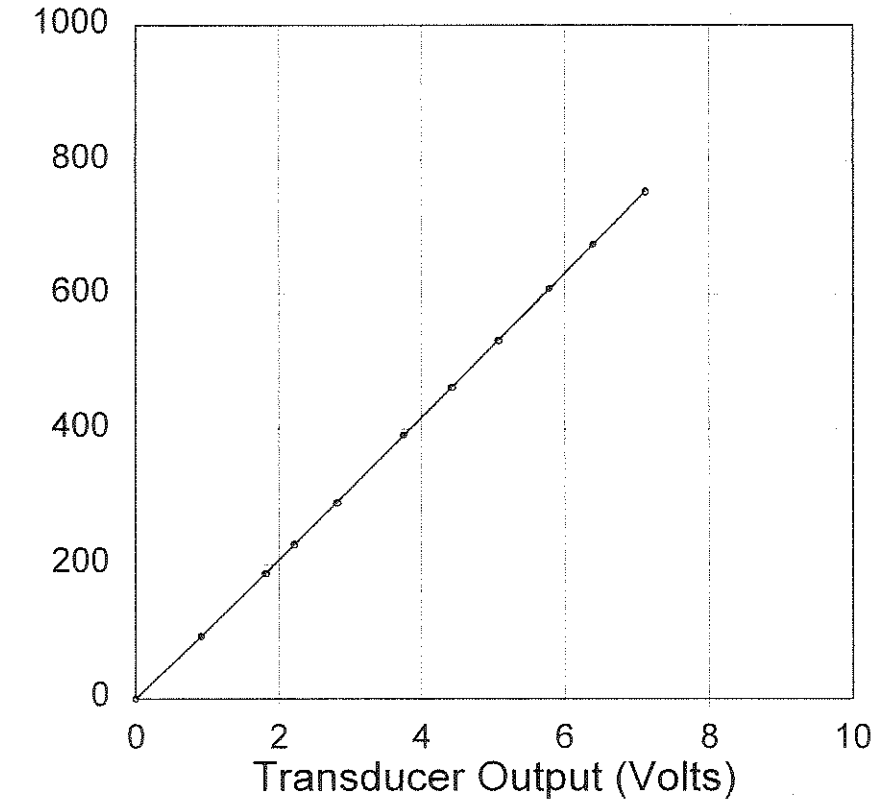

PDA Cal Factor 105.8με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
93	0.91
185	1.80
229	2.21
291	2.80
390	3.76
460	4.41
530	5.06
607	5.78
674	6.40
753	7.12

Shunt (60.4 KΩ) 5.0 V

General Factor 367.4με/mV/V

Traceable to N.I.S.T.

Calibrated by: J. Deutsch

Calibrated on: 21-Jun-2004

Strain Transducer Calibrator System 2004 Version 1.2