Pile Dynamics, Inc.

Transducer 480

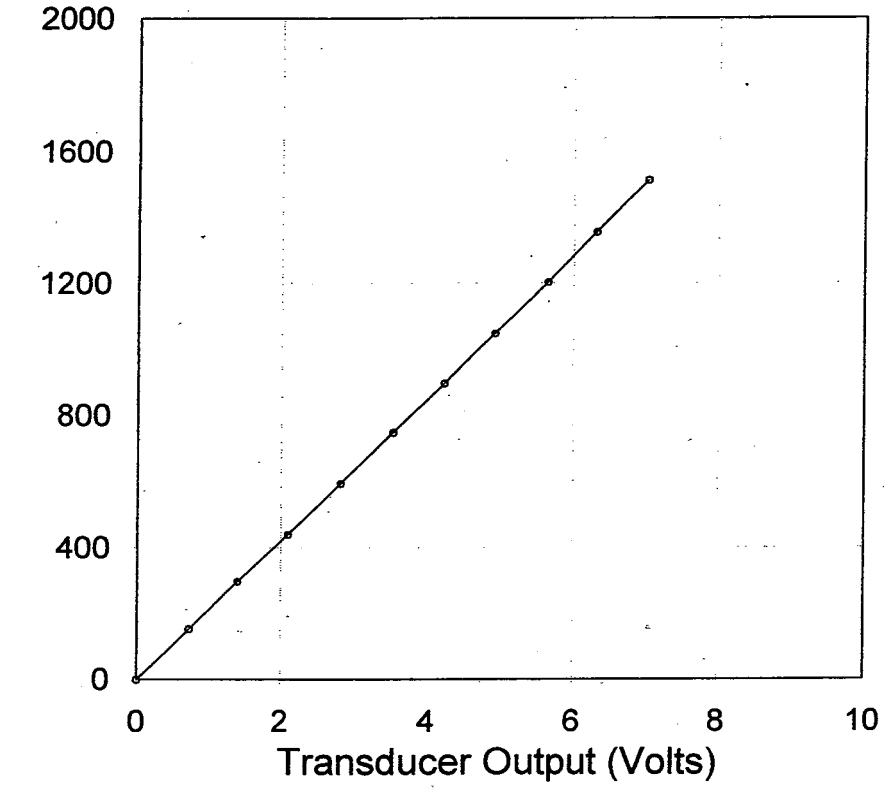

PDA Cal Factor (5.0 V) 107.4με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
154	0.72
297	1.40
439	2.10
593	2.82
748	3.53
895	4.22
1046	4.91
1202	5.63
1354	6.32
1513	7.03

Shunt (60.4 KΩ) 2.5 V

General Factor 372.8με/mV/V

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: MC

Calibrated on: 02-Oct-2014

Smart Sensor? ✓ Yes _____ No Smart Chip Programmed by: MJ Date: 10-2-14 CRC value 9923