


Pile Dynamics Inc Transducer 518F

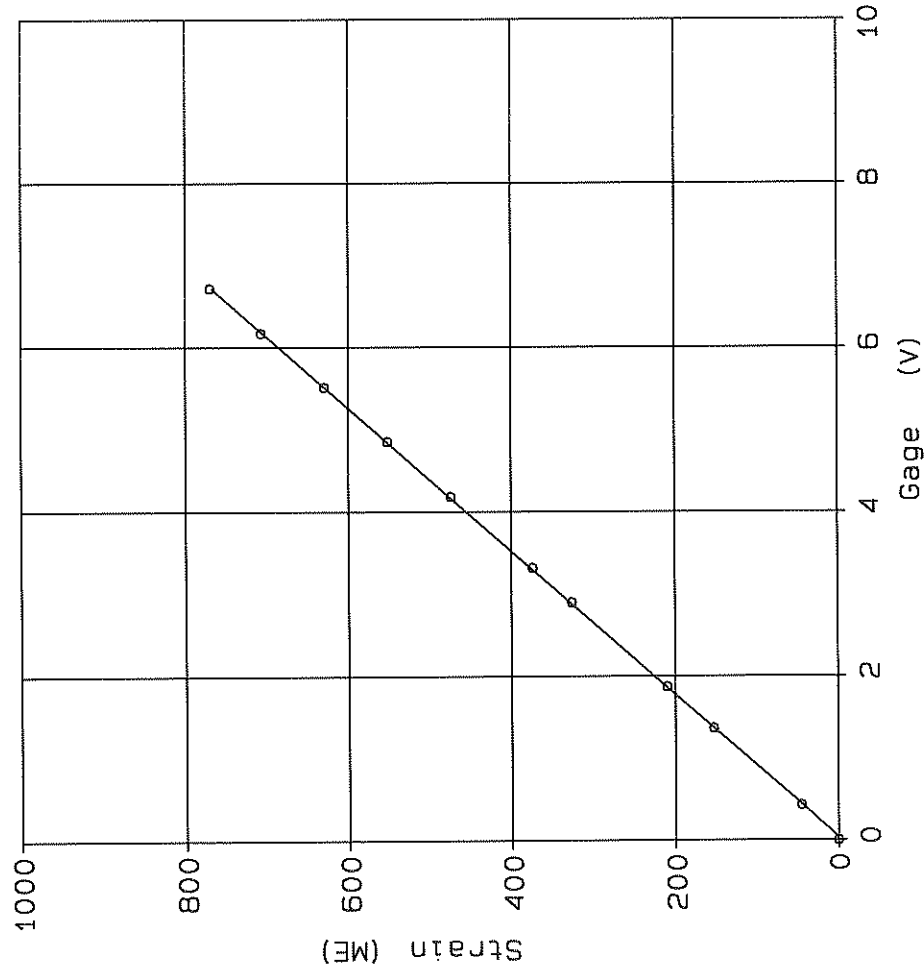

PDA Cal Factor = 114.7 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 398.4 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
46	.43
153	1.37
210	1.88
326	2.90
374	3.31
475	4.18
552	4.86
629	5.52
707	6.18
771	6.73

Calibrated by: J. S. Dantley

Calibrated on: 14-Jul-97