


Pile Dynamics, Inc. Transducer 563H

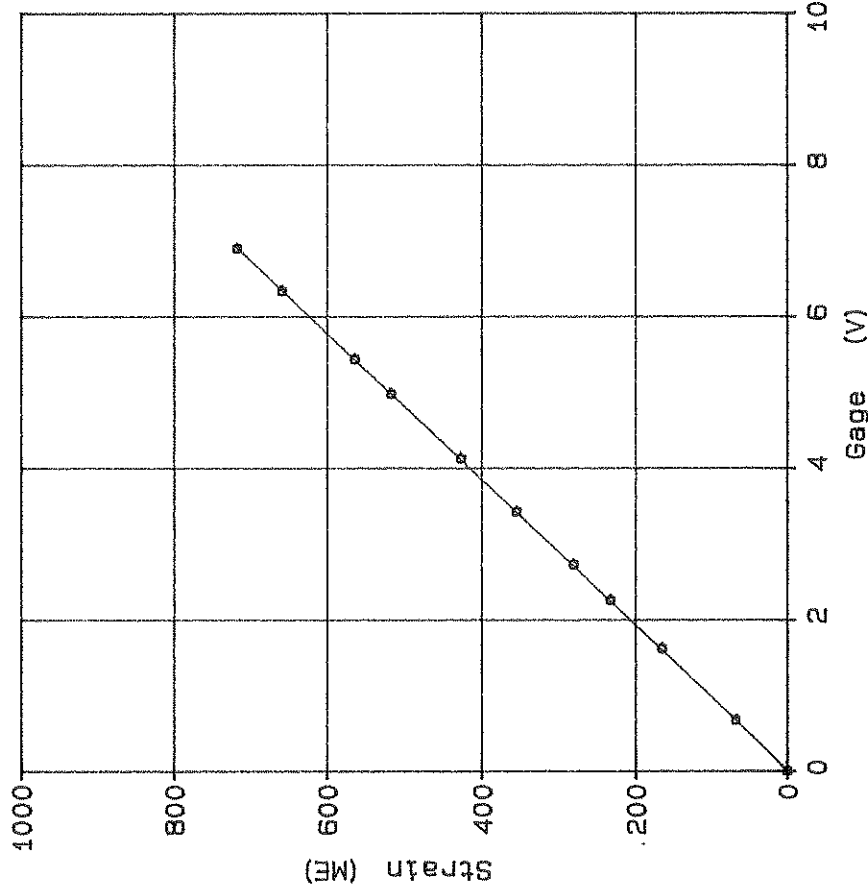

PDA Cal Factor = 104.0 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 361.2 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
70	.68
167	1.62
233	2.26
282	2.74
355	3.43
427	4.13
518	4.99
565	5.44
659	6.34
718	6.91

Calibrated by: Jim E. [Signature]
 Calibrated on: 07-Jun-94