


Pile Dynamics Inc Transducer 569H

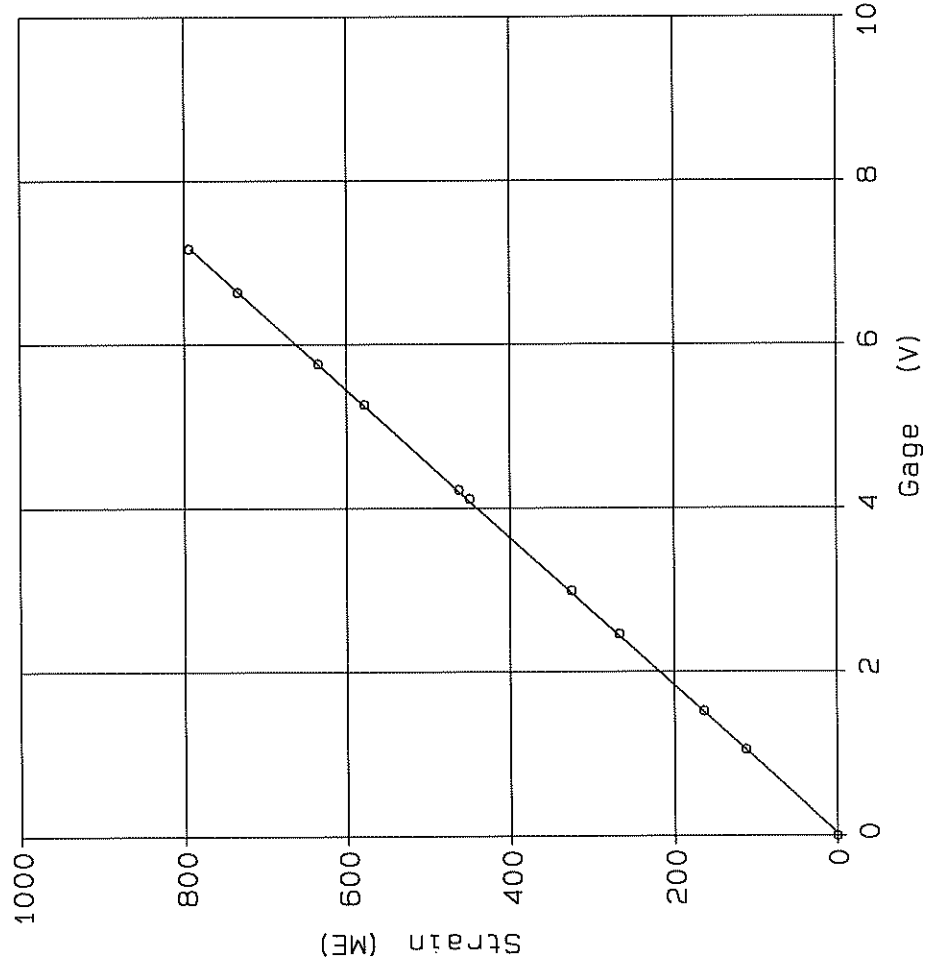

PDA Cal Factor = 111.0 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 385.3 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
113	1.05
164	1.52
268	2.47
326	2.99
450	4.11
462	4.22
579	5.26
635	5.76
735	6.64
795	7.18

Calibrated by: J. D. Bartlett

Calibrated on: 04-Aug-99