


Pile Dynamics Inc Transducer 576H

PDA Cal Factor = 90.1 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 313.0 ME/mV/V
 Traceable to N.I.S.T.

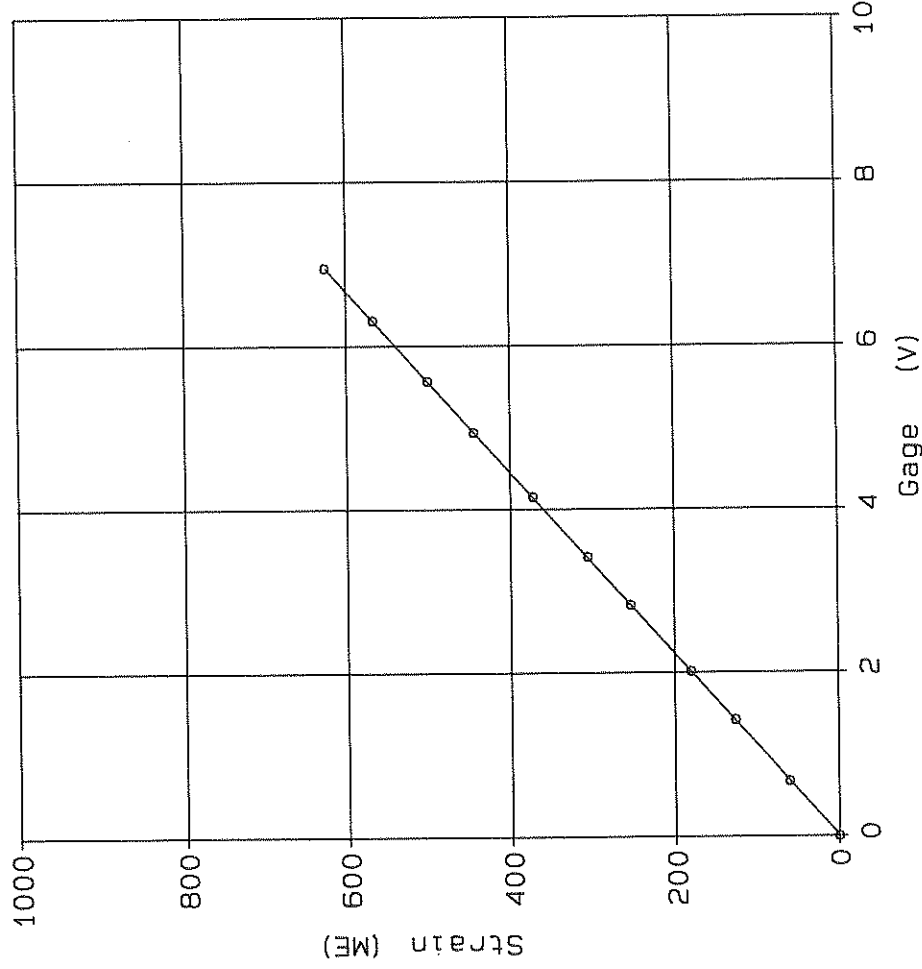

Strain ME	Gage V
0	.00
60	.68
127	1.43
180	2.01
253	2.82
306	3.41
373	4.15
445	4.95
501	5.58
568	6.31
627	6.95

J. J. Puntall

Calibrated by:

Calibrated on: 12-Mar-03