


# Pile Dynamics Inc Transducer 802H

PDA Cal Factor = 104.6 ME/V  
 Shunt (60.4K $\Omega$ ) = 5.0 V

General Factor = 363.1 ME/mV/V  
 Traceable to N.I.S.T.

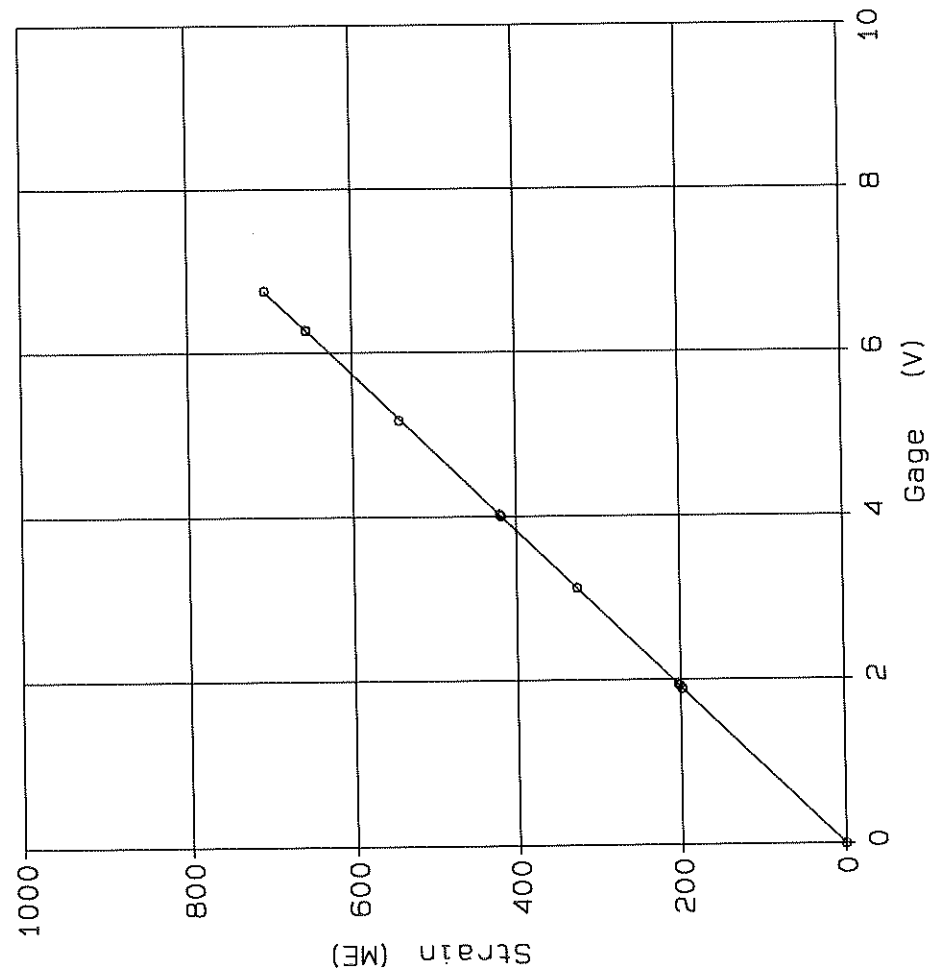

| Strain<br>ME | Gage<br>V |
|--------------|-----------|
| 0            | .00       |
| 204          | 1.96      |
| 202          | 1.93      |
| 198          | 1.90      |
| 326          | 3.12      |
| 421          | 4.02      |
| 419          | 4.00      |
| 543          | 5.18      |
| 657          | 6.28      |
| 656          | 6.28      |
| 707          | 6.76      |

Calibrated by: *J. C. Anthony*

Calibrated on: 07-Nov-01