




Pile Dynamics, Inc.

Transducer 803H

Strain ($\mu\epsilon$)

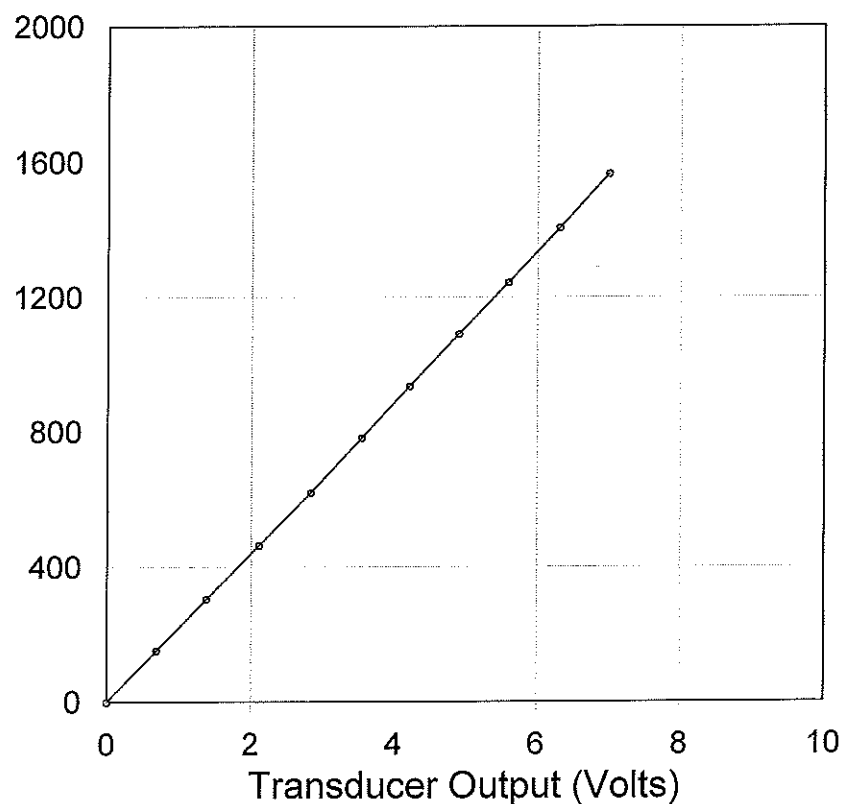

PDA Cal Factor (5.0 V)

111.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
153	0.69
304	1.38
463	2.11
617	2.83
781	3.53
935	4.21
1089	4.90
1244	5.59
1405	6.31
1565	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

387.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by:

Erin S. Smith

Calibrated on:

22-Aug-2012