




# Pile Dynamics, Inc.

Transducer 8093

Strain ( $\mu\epsilon$ )

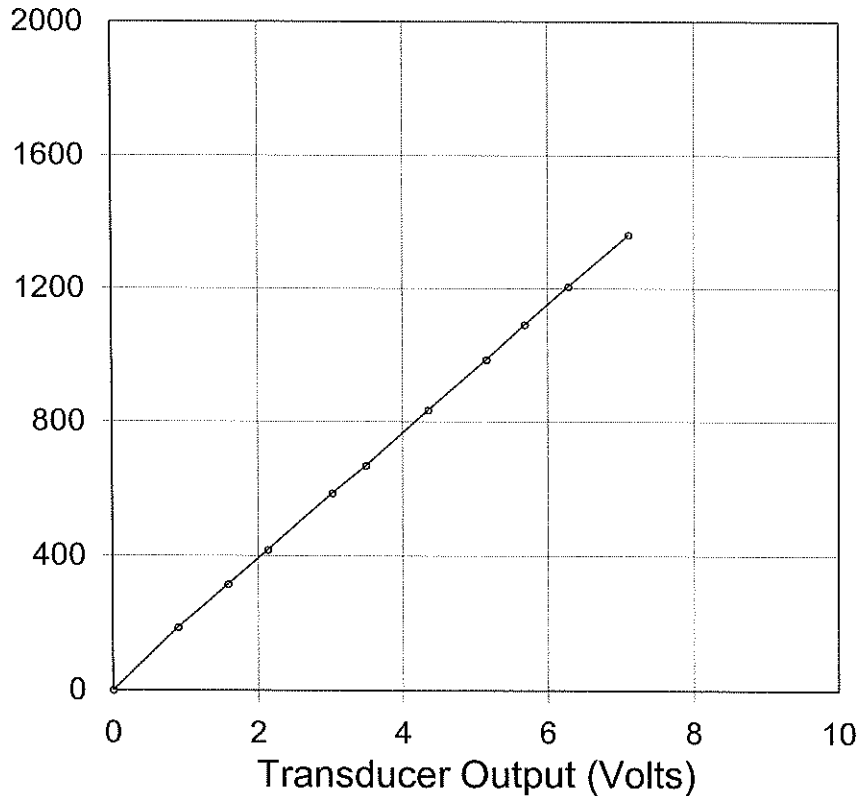

PDA Cal Factor (5.0 V)

95.2 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
187	0.90
316	1.59
417	2.13
585	3.02
668	3.48
834	4.35
986	5.15
1092	5.68
1207	6.28
1362	7.10

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

330.5 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

07-Jun-2007