




Pile Dynamics, Inc.

# Pile Dynamics, Inc.

## Transducer

## 8096

Strain ( $\mu\epsilon$ )

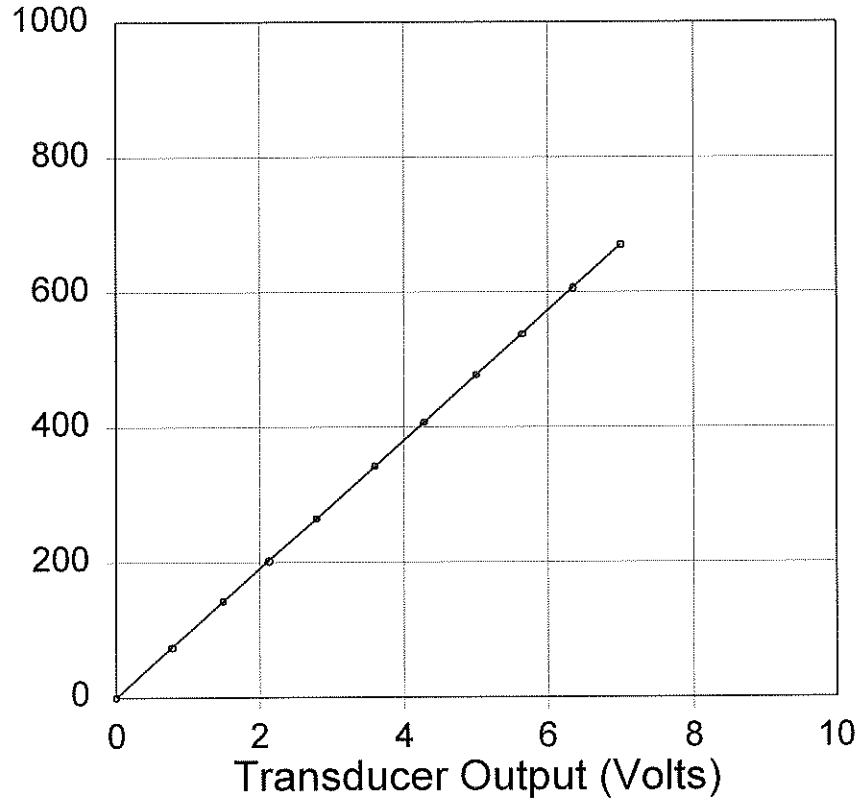

PDA Cal Factor

95.6 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
74	0.77
143	1.49
202	2.12
263	2.78
342	3.59
406	4.27
476	5.00
538	5.64
606	6.34
670	7.00

Shunt (60.4 K $\Omega$ )

5.0 V

General Factor

331.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2003 Version 1.1

Calibrated by:

Calibrated on:

29-Dec-2003