

Pile Dynamics, Inc.


Pile Dynamics, Inc.

Transducer

8099

Strain ($\mu\epsilon$)

1000

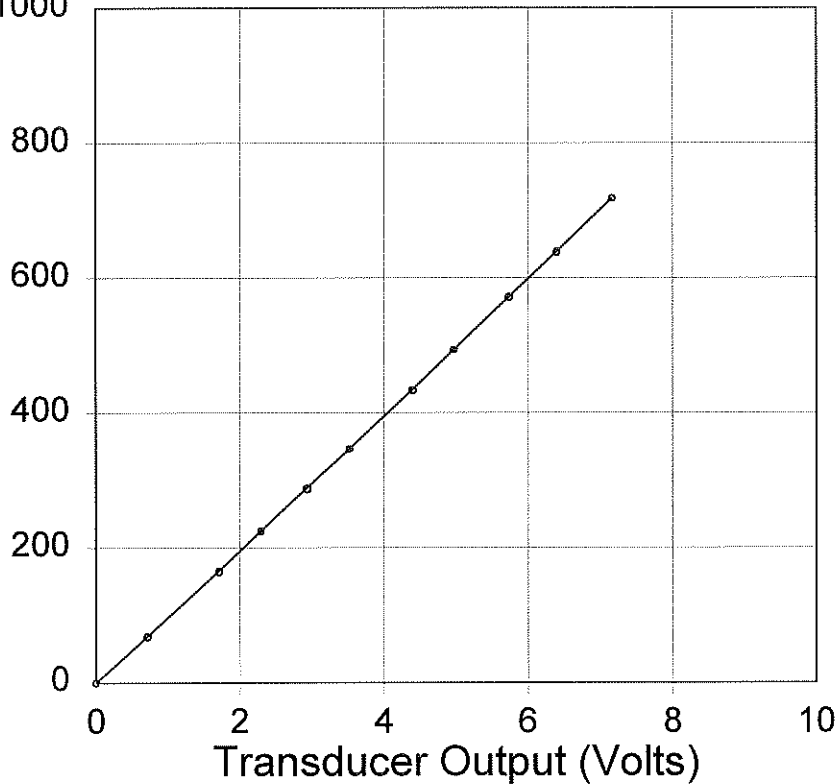

PDA Cal Factor

100.5 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
69	0.71
166	1.70
224	2.29
287	2.92
346	3.51
433	4.38
492	4.96
571	5.73
640	6.40
719	7.15

Shunt (60.4 K Ω)

5.0 V

General Factor

348.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2003 Version 1.1

Calibrated by:

Calibrated on:

05-Jan-2004