




Pile Dynamics, Inc.

Transducer 8101

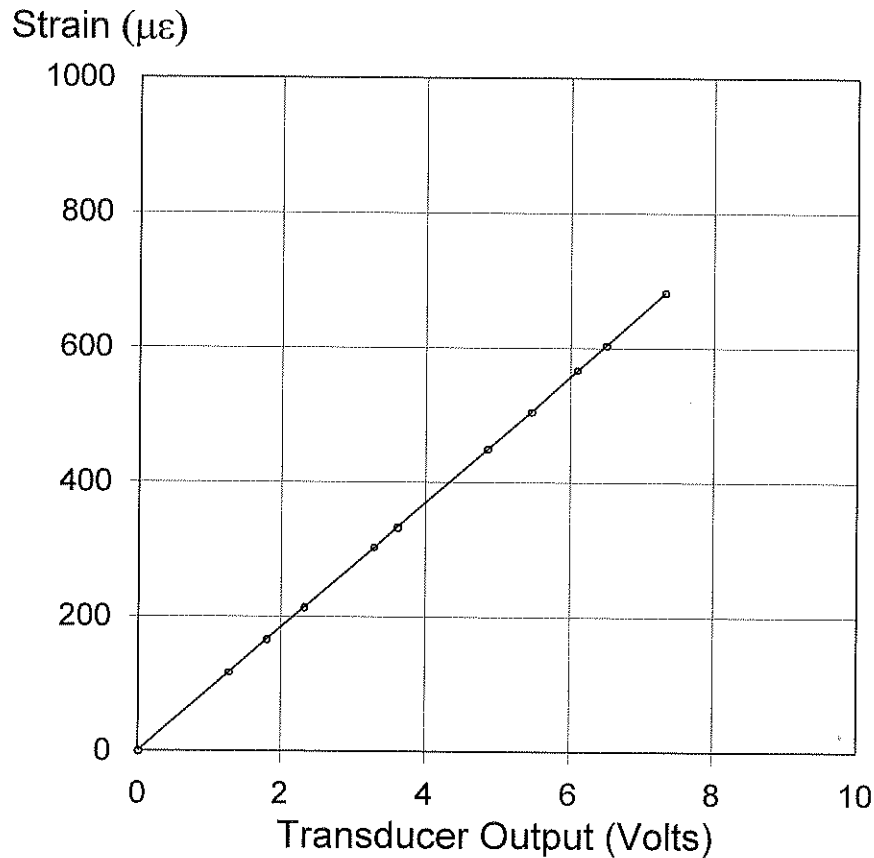

PDA Cal Factor 93.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
117	1.26
166	1.79
214	2.32
303	3.28
333	3.60
449	4.85
505	5.45
566	6.09
603	6.49
682	7.32

Shunt (60.4 K Ω) 5.0 V
 General Factor 323.5 $\mu\epsilon/mVV$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by: *R Eason*
 Calibrated on: 25-Oct-2004