




Pile Dynamics, Inc.

Transducer 8103

Strain ($\mu\epsilon$)

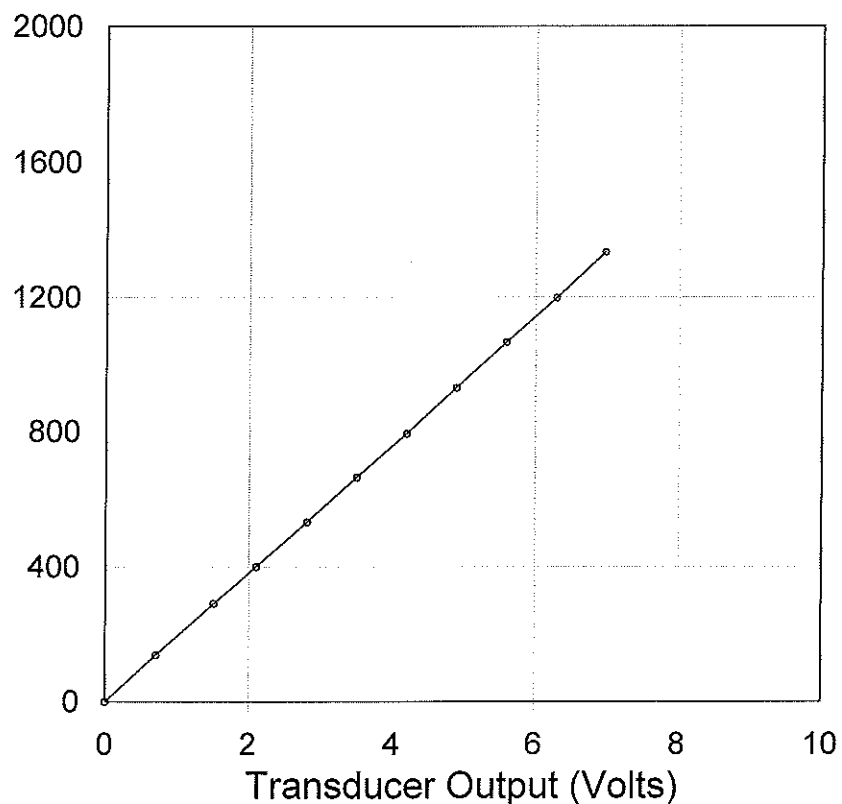

PDA Cal Factor (5.0 V)

95.3 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
140	0.71
292	1.51
400	2.10
532	2.80
663	3.49
794	4.19
930	4.89
1065	5.59
1199	6.28
1334	6.97

Shunt (60.4 K Ω)

2.5 V

General Factor

330.9 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Calibrated by:

Emp. Smith

Calibrated on:

24-Sep-2012