




# Pile Dynamics, Inc.

## Transducer 8121

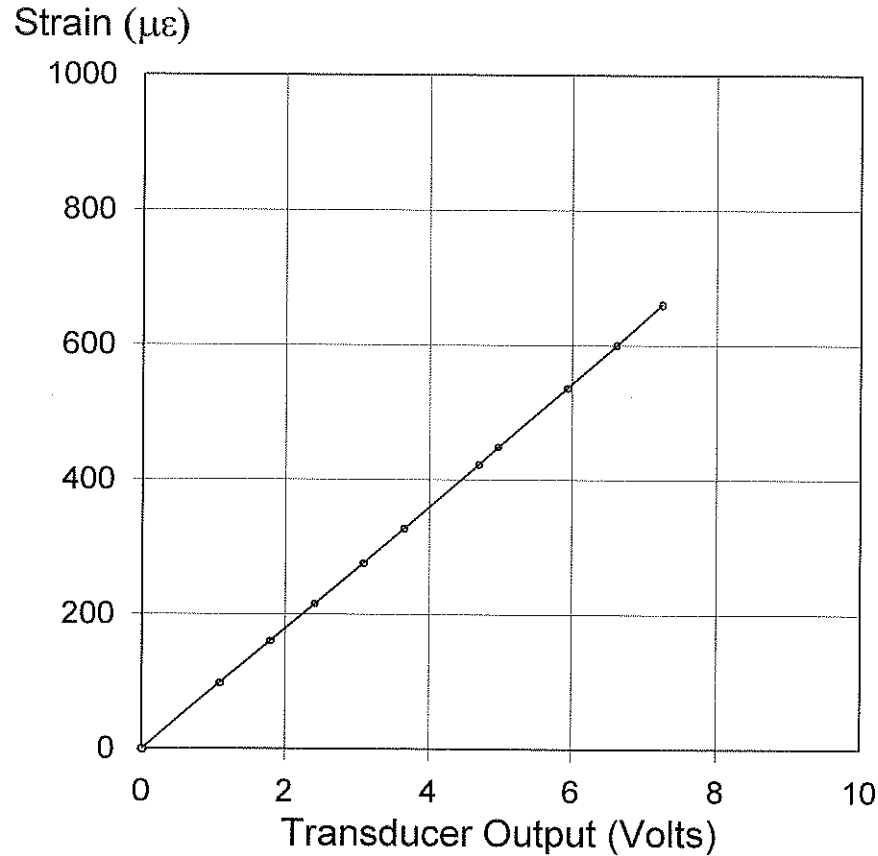

PDA Cal Factor 91.0 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
98	1.09
160	1.78
215	2.40
276	3.08
328	3.65
422	4.69
448	4.96
536	5.92
600	6.61
661	7.25

Shunt (60.4 K $\Omega$ ) 5.0 V  
 General Factor 316.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by: Fred Harris  
 Calibrated on: 08-Sep-2005