


Pile Dynamics, Inc.

Transducer 8122

Strain ($\mu\epsilon$)

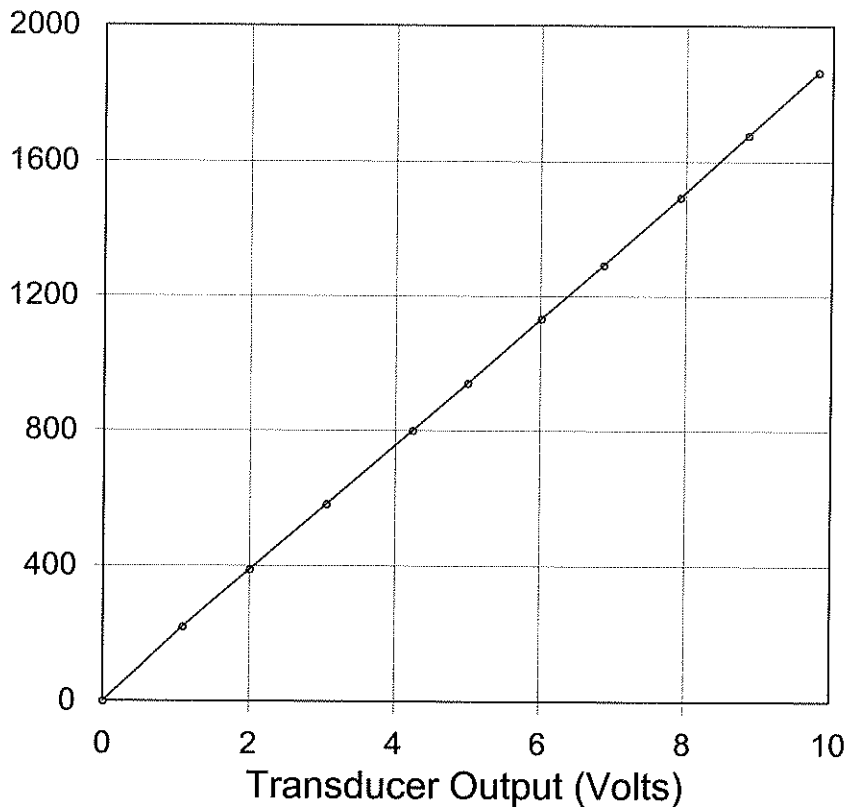

PDA Cal Factor (5.0 V)

94.3 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
219	1.08
389	2.00
580	3.05
799	4.23
939	4.99
1133	6.01
1294	6.87
1494	7.93
1678	8.85
1865	9.81

Shunt (60.4 K Ω)

2.5 V

General Factor

327.4 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:


04-Jun-2007