


Pile Dynamics, Inc.

Transducer 8124

Strain ($\mu\epsilon$)

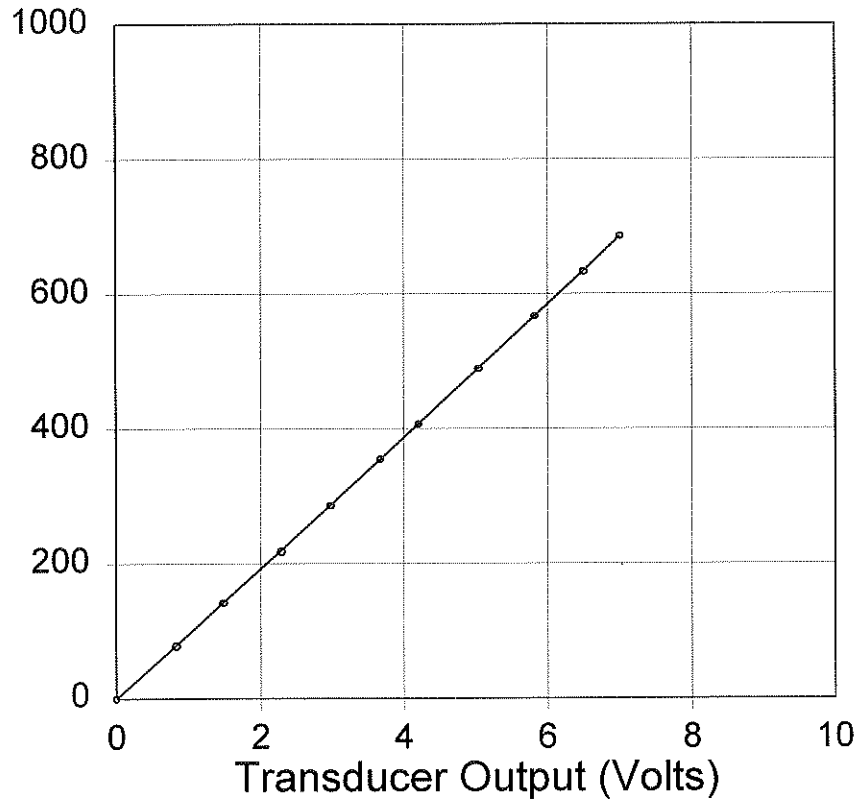

PDA Cal Factor

98.0 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
78	0.82
141	1.47
218	2.27
285	2.97
355	3.67
406	4.20
488	5.03
567	5.82
634	6.49
686	7.00

Shunt (60.4 K Ω)

5.0 V

General Factor

340.2 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2003 Version 1.1

Calibrated by:

Calibrated on:

B. Eason
05-Jan-2004