




# Pile Dynamics, Inc.

## Transducer 8129

Strain ( $\mu\epsilon$ )

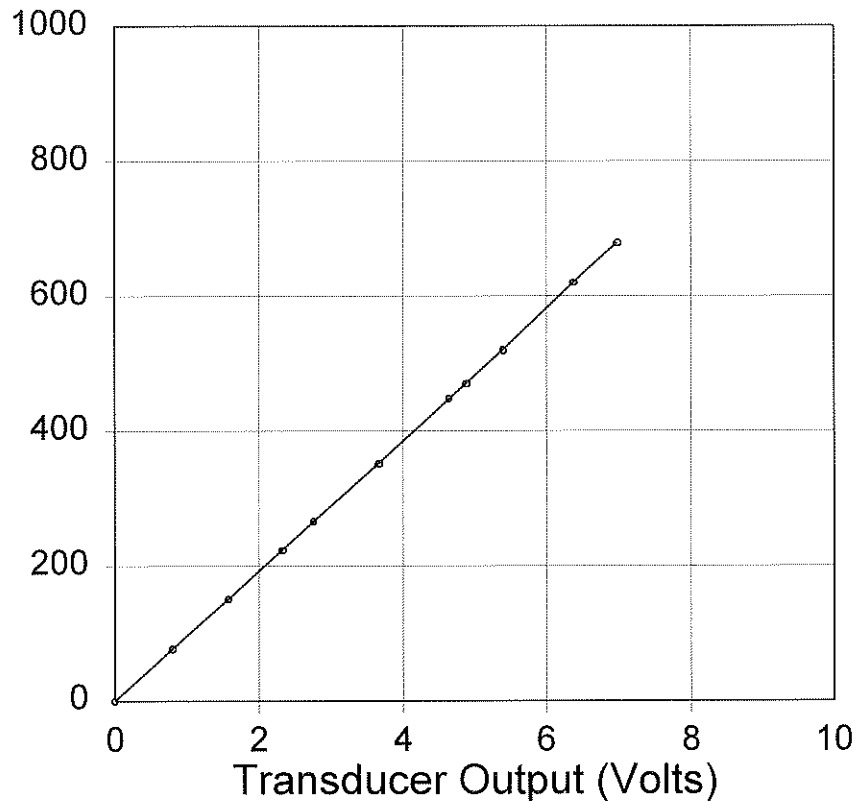

PDA Cal Factor

97.1  $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
77	0.80
151	1.57
223	2.32
265	2.76
352	3.65
447	4.64
470	4.87
520	5.38
619	6.38
679	6.98

Shunt (60.4 K $\Omega$ )

5.0 V

General Factor

337.3  $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

*R Eason*  
25-Feb-2004